



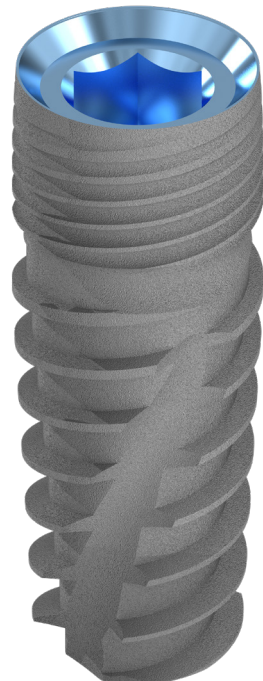

BIOLEVEL

IMPLANT SYSTEM

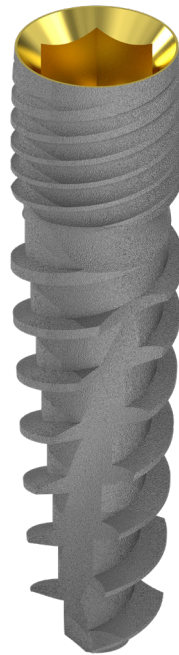

BIOLEVEL

The most complete solution a doctor can give to a patient

TABLE OF CONTENTS

INTRODUCTION

About the company	3
Technology and quality	4
Implant surface finish, raw materials	6
Packaging	8

BIOLEVEL IMPLANT SYSTEM






The distinctive characteristics of the BIOLEVEL system	12
The functional structure of the system elements	14
The applicational fields of BIOLEVEL	15
Implants with a Ø 2.75 platform	16
Implants with a Ø 3.00 platform	18
Implants with a Ø 3.50 platform	20
Implants with a Ø 4.55 platform	22
Implants with a Ø 5.70 platform	24
	26

BIOLEVEL ABUTMENT SYSTEM

Sizes available of the abutments	28
	32

INSTRUMENTS

Large instrument kit	38
Small instrument kit	40
Surgical drills	42
Ratchet torque wrench	44
	46

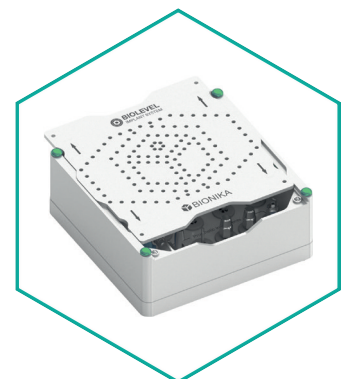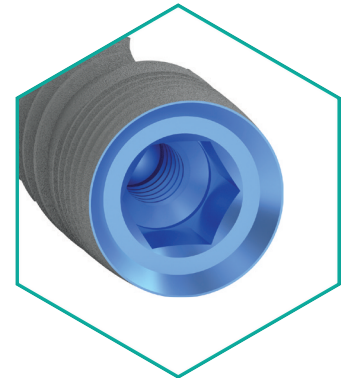



About the company

Bionika Medline Kft. was established in 1989 by private individuals as a family-owned Hungarian company. We have more than 35-year-experience in the field of medical instruments and implant development, production and trade.

According to our objective and perception, we attach great importance to the word "BIONIKA", which marks a scientific thinking on the boundaries of biology, technology and electronics that combines these three areas in our researching and developing work.

Clinical and technological experiences: The continuous process, combination and utilization of clinical and technological experiences in development contributes to our success, up to the production base. Here you will find the best solutions and constructions suited to customer needs, which are under continuous development.


Development: The owners of BIONIKA put great emphasis on continuous product and technological research and development. Our products are developed in close collaboration with doctors and engineers, enabling us to ensure the world-class quality and practical utilization.

Quality: The quality of the products expected by our customers is guaranteed by design, manufacturing and quality management according to the harmonized European Union laws. The BIONIKA Medline Kft. is operated according to the EN ISO 9001 and the EN ISO 13485 quality management system. Our products are provided with CE marks.

Guarantee: After inserting the implant - the risk of the ossification process is assumed by BIONIKA, independently of cause and effect relationship – exchange guarantee is ensured within one year after the purchase. Otherwise, we provide a long-term, 10-year guarantee for our products.



DENTISTRY



ORAL SURGERY



TRAUMATOLOGY



ORTHOPEDICS

Technology

BIONIKA Medline Kft. has more than 35 years of experience in the development and production of dental implants, dental insertion instruments and stomatological parts. During this time more than 40 types of implant systems have been developed and are being manufactured to date, including insertion instruments.

Some of these parts have been developed for their own marketing in accordance with their own market needs. Other systems - in cooperation with independent medical groups - are made to order, mainly developed and manufactured for foreign markets. (These are sold by the customers under their own brand name).

Our partners can choose from approximately 20.000 different parts of different sizes and shapes. Our manufacturing technology is flexible, we can quickly move from one component to another, and we are able to fulfill thousands of orders with a short turnaround time.

This area requires high precision production (in some cases it is necessary to hold 2-5µm tolerances). All the technological operations we carry out are from manufacturing, surface design, packaging. Our products are

CE marked and the production process is under strict quality management system.

Biocompatible materials are the most important raw materials for dental, oral surgery, traumatology and orthopedic medical implants.

Because relatively small series of customized solutions are required, they require fast programmable CNC machining technology. Accordingly, we have molded CNC machining centers and Swiss type longitudinal machining centers. For machining more complex surfaces, an industrial 5-axis CNC center is used with CAD-CAM system support. Our machines are equipped not only with fixed, but also with propelled cutting instrument units, with which we can perform more complex spatial geometrical machining.

As a complementary technology, we have sandblasting, polishing titanium coloring and sterilization equipments.

The production of custom prosthetic components for dental applications is supported by the BIONIKA Milling center.

Our Partners



Quality management and guarantee

The quality of the products is guaranteed by design, manufacturing and quality management according to the harmonized European Union laws. The BIONIKA Medline Kft. is operated according to the EN ISO 9001 and the EN ISO 13485 quality management system. Our products are provided with CE marks, which was ensured by EMKI and QT-CERT.

We provide a long-term, 10-year guarantee for our products. After inserting the implant, reducing the medical risk of the ossification process, independently of cause and effect relationship – exchange guarantee is ensured within one year after the purchase for the dropped and fallen out implants.



BIONIKA Medline Kft. has always paid close attention to quality and reliability during its more than 35 years of existence. The Bisnode certificate is proof of our reliability and stability. BIONIKA received "Triple A" Bisnode qualification from 2016 to 2024.

At the Hungarian market only 0.63% of the companies have the AAA Bisnode rating. The financial risk of establishing business relationship with these business associations is extremely low - source: dnb.hu

Superclean Implant Surface

BIONIKA demonstrates the best qualities of Grade 4 titanium used in implant manufacturing for dental implantology according to the ISO 5832-2 ASTM F67 standard.

Due to its adequate purity the biocompatibility is exceptionally good as well as it is provided with exceptional solidity. Initially, we and other implant manufacturers preferred the higher purity titanium but due to solidity reasons nowadays almost every implant is made of Grade 4 or other alloyed titanium in the world.


In all cases of implant abutments, alloyed, high strength Grade 5 titanium is applied according to the ISO 5832-4 ASTM F136 standard. The titanium applied according to the standard is provided with exceptional biocompatibility, it is almost risk-free. Almost all professionals see that the implantation success is best determined by the implantologist's practice, as well as surgical conditions, carefully maintained hygiene, and patient abilities.

The main steps of our **BioTiS surface finish technology**:


- Chemical, mechanical surface cleaning and surface dewing
- Special ultrasonic cleaning, surface cleaning and sterilization
- Transformation of surface structure by acidification process
- Multi-stage dehumidification, cleaning
- Electrochemical surface modification
- sterilization
- Surface finish in physiological solution

These technological steps are always carried out under sterile conditions.

The final packaging of the implants is four-layered. The packaging is carried out in a sterile cabin. Final sterility is assured by an accredited 20 Rad gamma sterilization procedure.

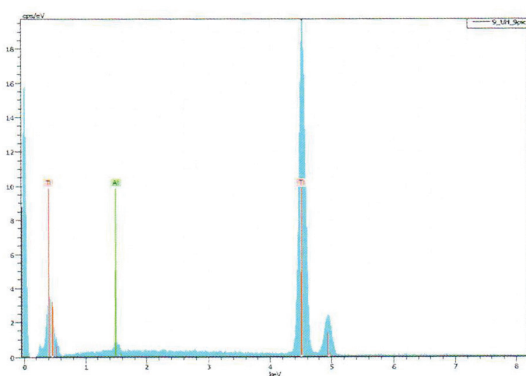

Energy dispersive X-ray spectrometric elemental analysis of Bionika implants*

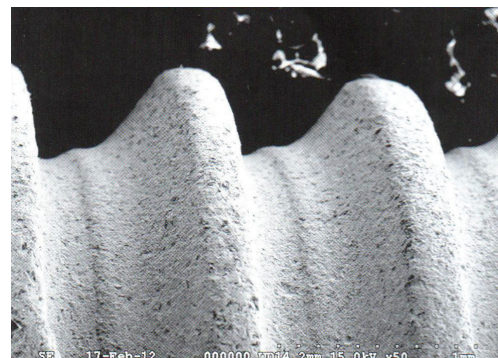

Bionika implant electron microscope image *



Bionika implant electron microscope image *

* Source: FOGORVOSI SZEMLE, year 106. No. 4 2013. 135-143

Applied raw materials

Titanium grade 4

Chemical composition

Elements	Threshold limit of constituents(%)
O	0,4 max.
Fe	0,3 max.
C	0,1 max.
N	0,05 max.
H	0,0125 max.
Ti	>99% / balance

Mechanical properties

solidity	680 MPa min.
dilation	10 %

According to the **ISO 5832-2** standard.



Titanium Grade 5

Chemical composition

Elements	Threshold limit of constituents(%)
Al	5,5-6,75 max.
V	3,5-4,5 max.
Fe	0,3 max.
O	0,2 max.
C	0,08 max.
N	0,05 max.
H	0,015 max.
Ti	balance

Mechanical properties

solidity	860 MPa min.
dilation	10 %

According to the **ISO 5832-3** standard.

CoCr

Chemical composition

Elements	Threshold limit of constituents(%)
C	0,1 max.
Si	1,0 max.
Mn	1,0 max.
P	0,005 max.
S	0,005 max.
Cr	30, 0 max.
Mo	7,0 max.
Ni	1,0 max.
Co	-
N	0,2250 max.

Mechanical properties

solidity	1240,00 MPa min.
elongation limit	900,00 min.
elongation at break	18,00 min.
fracture contraction	23,00 min.

According to the **ISO 5832-4** standard.

Plastics

POM (polyoxymethylene) : Thermoplastic synthetic plastic, Excellent properties eg: high hardness, low wear, good flexibility, little absorbing ability. Density: 1.41 g / cm³. elongation at break: min. 30% Current Voltage: min. 65 Mpa. Its color is white.

PEEK (polyether ether ketone) :High heat-resistant plastic, suitable for all conventional sterilization methods (steam, dry heat, ethylene oxide, gamma radiation). Density: 1.30 1.41 g / cm³ Tensile strength: 115 Mpa. elongation at break: min. 17% Its colour is natural brownish gray.

BIOLEVEL packaging



10-piece collection box



vial in sterile foil



removing the foil



sterile vial



removing the locking
plug (1)



removing the locking
plug (2)



the implant and the multifunctional
head in the locking plug



using the implant key driver



Collection box

Depending on the order quantities, collection boxes with 5 and 10 pieces are applied.

BIOLEVEL Packaging



Vial

The first layer of the packaging is a transparent vial, this ensures the total, null colony-forming unit sterility. The locking plug of the vial holds the implant, the multifunctional head and the locking screw.

Biolevel, Normál Implantátum
 Ø 4,25 x L13,00 mm
 REF 500.002.425.130 2016-06
 LOT 121214-08 2021-06
 CE 1008 2 STERILE R CM 007
 BIONIKA Medline Kft.
 3516 Miskolc Tégla u. 29. www.bionika.hu

Paper box

The outer layer of the packaging is a paper box with a high density, which is for the physical safety. Every paper box is provided with colour-coded labels according to the different platform- diameters. The colour of the packaging is adjusted to this method.




The sectional image of the **BIOLEVEL** packaging and its accessories






The first layer of the packaging is a transparent vial. The implant and the multifunctional head are held by the vial locking plug and with this they can be removed from the vial. The implant locking screw can be found in the vial locking plug as well.

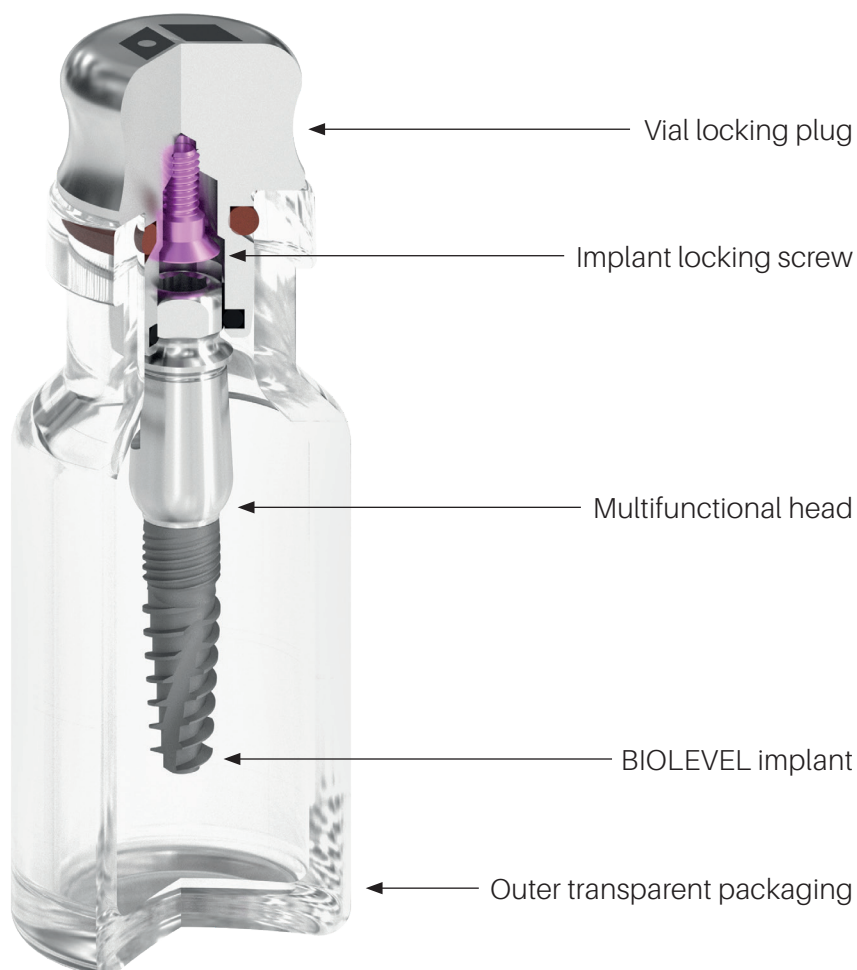The **multifunctional head** doesn't only hold the implant in the packaging but also helps its inserting into the jaw bone, is suitable for closed spoon sampling and after this it can be drilled as a head for the glued toothwork.



BIOLEVEL product labels and their notation

Differential platform sizes by colour and diameter (mm):


 2,75 mm - grey
  3,0 mm - yellow
  3,5 mm - purple
  4,5 mm - blue
  5,7 mm - green

Information supplied by the three product labels to the outer packaging of the Implant System:


The side of the box:




Top of the box:

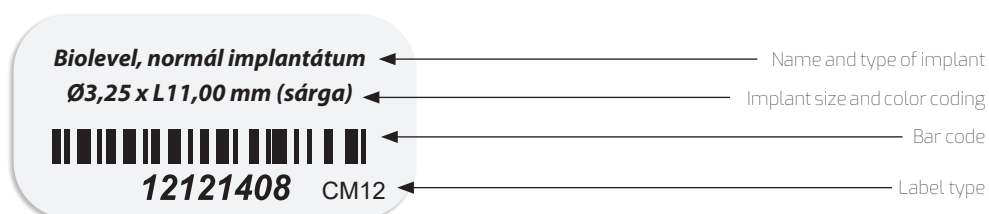



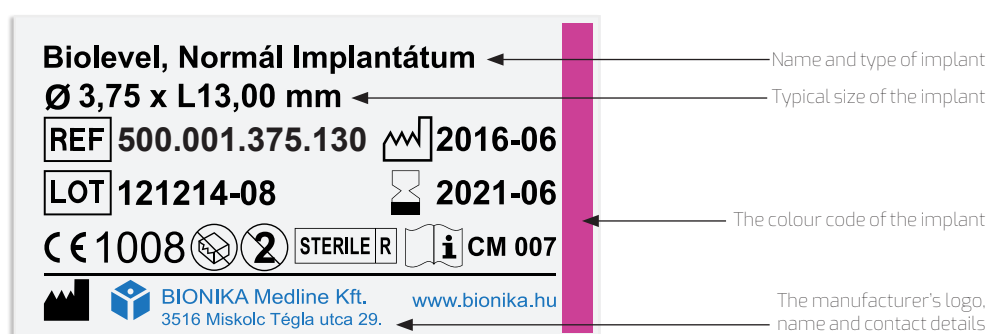

The back of the box:



Explanation of label codes:

Ø	Diameter
L	Implant length
REF	Item number
LOT	Serial number
	Production time

	Expiration date
	It is forbidden to use in the case of damaged packaging.
	Reuse is forbidden!
STERILE R	Sterilized with gamma rays
STERILE 	sterilized with steam or dry heat

	Non-sterile product in the package
	Read the usage guide!
CE 1011	Certification company code
	Manufacturer's name and Contact




IMPLANT SYSTEM | TABLE OF CONTENTS

Distinctive characteristics	14
The applicational fields of BIOLEVEL	16
Sizes available of the implants	18




The distinctive characteristics of the **BIOLEVEL** Implant system

A demand was raised for a wide range of compatibility of dental implants during the dental and implantological practice. Thus the BIOLEVEL implant family was developed, which brought a significant change in the case of the implanting tools and abutments.

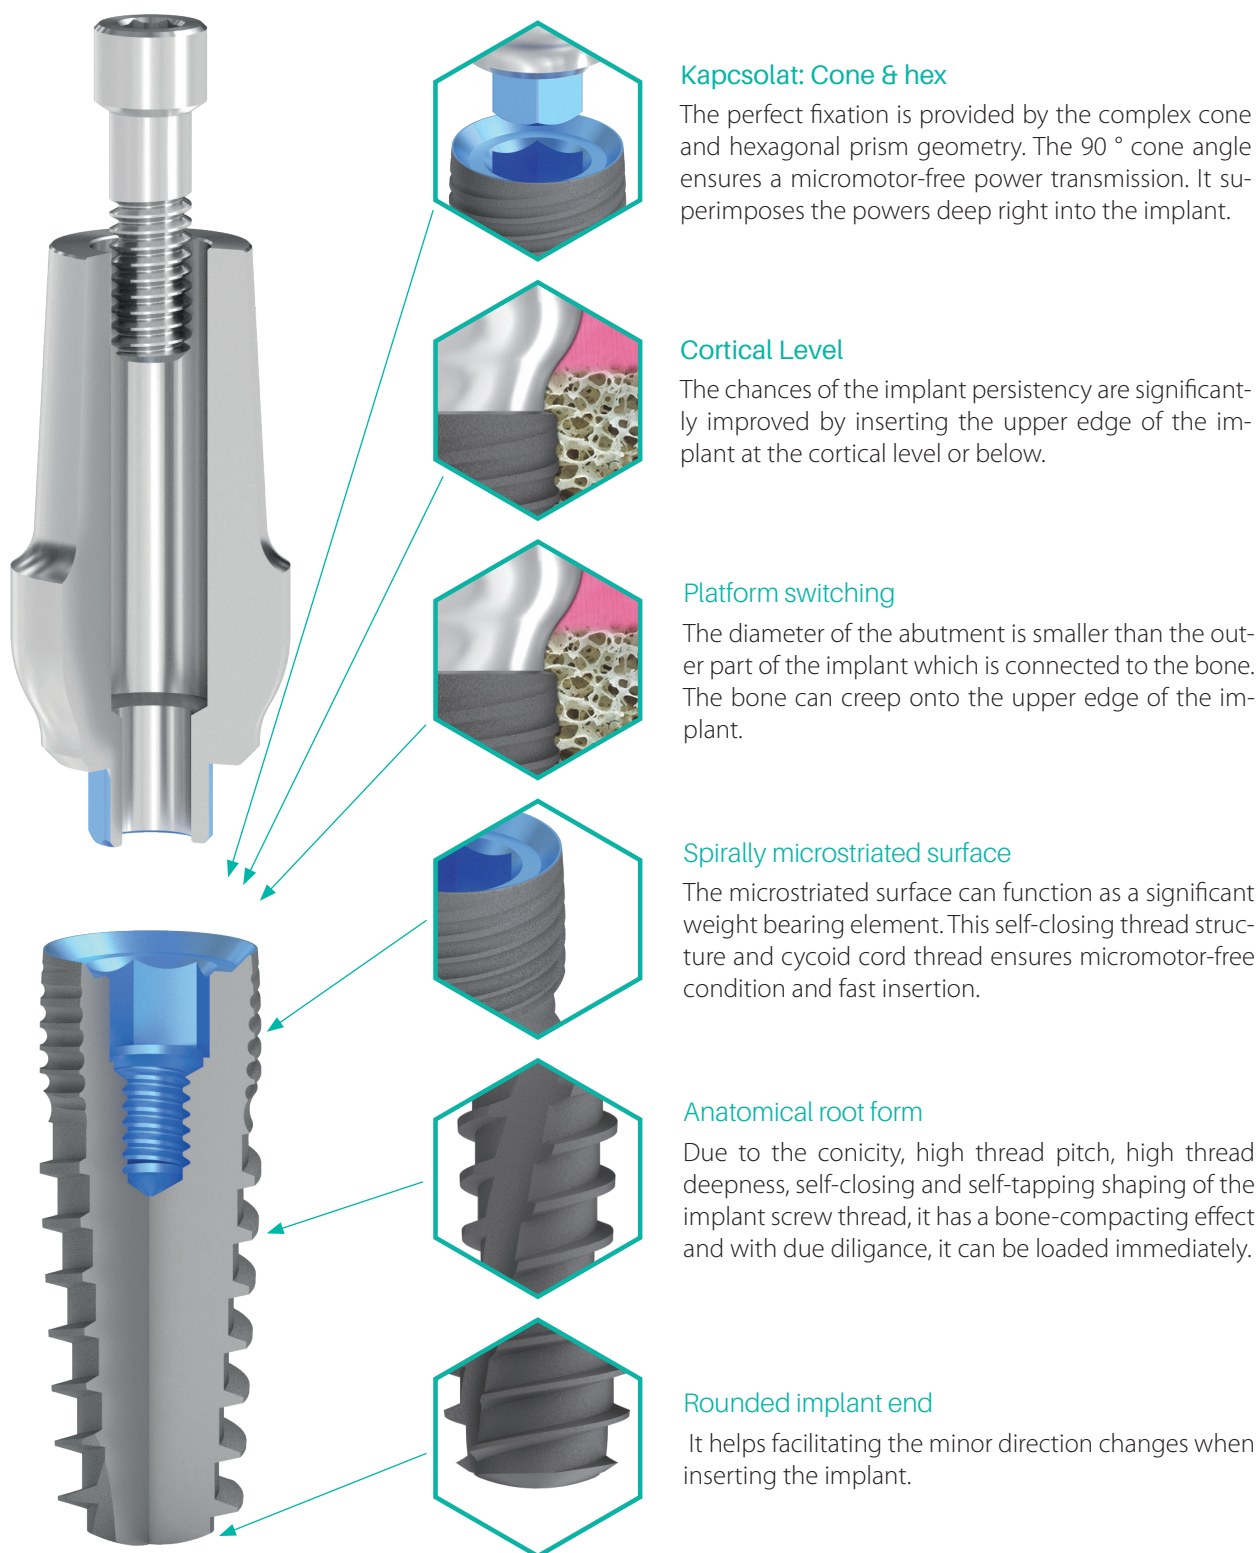

The functional structure of the BIOLEVEL system elements

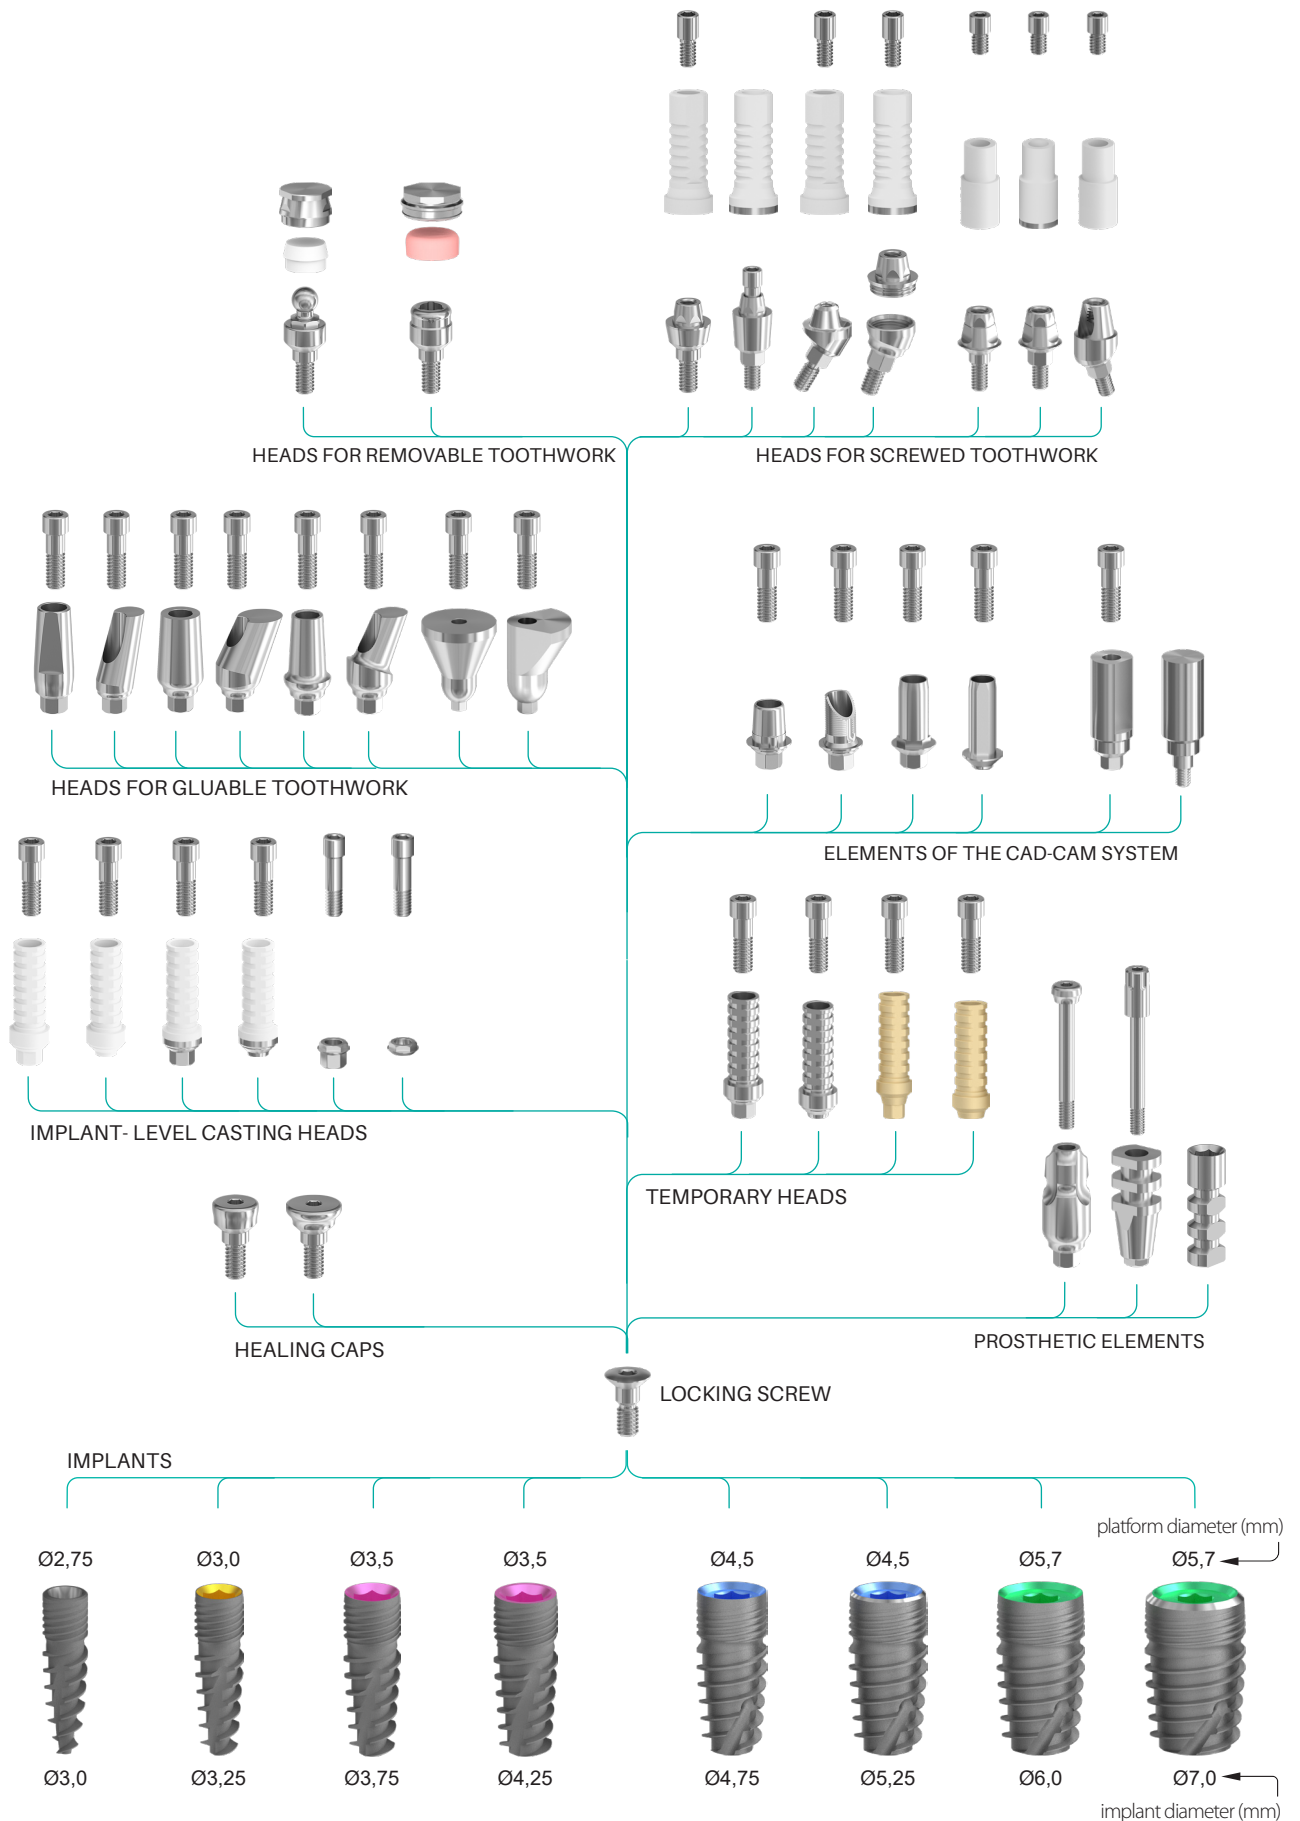

The applicational fields of the BIOLEVEL system




In the case of one tooth deficit

In this case of the replacement of a tooth, we do not have to grind two healthy teeth for bridge replacement, but inserting an implant, then we need to glue a crown in the same way as the traditional one.

In the case of end of line tooth deficit(s)

In this case, in the absence of a pillar tooth, we are not able to make a fixed replacement (bridge). With the implantation of at least two implants, you are already make the (fixed) bridge replacement.

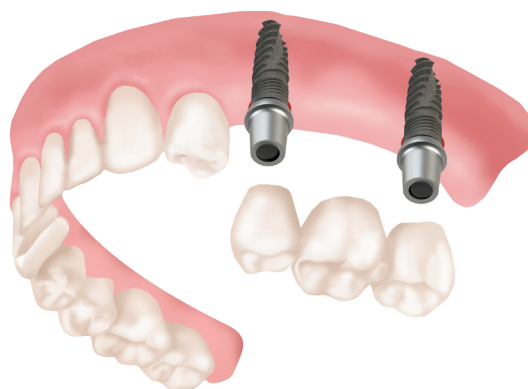

Removable denture


In the case of total tooth deficit

In this case the patient has no tooth, complete tooth augmentation can be performed. In this case, there one solution is the removable denture: 2-4 implants are implanted, these will be the fixation for the removable tooth.

This brings a tremendous quality of life to the patient, as this way the denture will be very stable, so it can be used in chewing and speaking outright.

There are two solutions possible in this case: ball head or locator head abutments can be applied. With the implantation of several 6-8 implants, it is possible to make full fixation (round bridge) augmentation, which is both functional and aesthetically close to the natural teeth.

Screw-retained fixed dental prosthetics

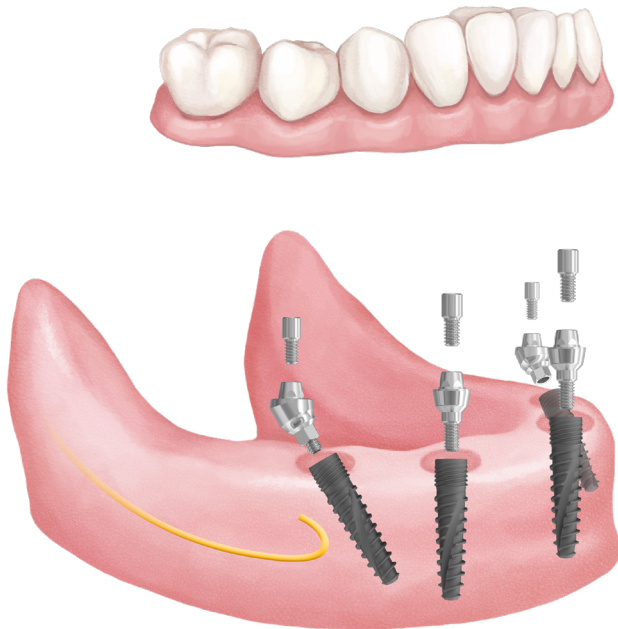

Optimum Concept

Optimum Concept

All-on-4® type - Economical Solution

The Optimum Concept provides great stability, with only four implants being implanted.


- The temporary denture can be inserted on the day of surgery.
- Immediate improvement in function, speech and aesthetically.
- Treatment times are shorter and costs can be lower than conventional implant placement modes.
- Tilt rear implants can be fixed better into the front bone. This promotes prosthesis support.

Safe Concept

All-on-6® type - For extra stability


The stability of the toothwork can be increased with the Safe Concept. It is exceptionally advantageous in the case of extra chewing ability.

- The usage of oblique head implants allows longer implants to be used, avoiding the nerve canal.
- The usage of longer implants allows the bone and the implant to touch on a larger surface, thus making bone augmentation avoidable.
- Favorable bone level for tilted and axial implants.
- High remaining chances.

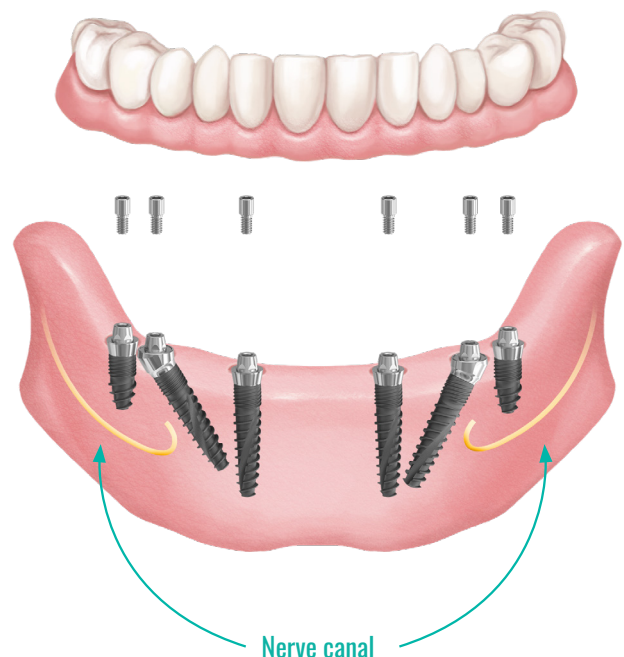


Safe Concept

BIOLEVEL implants with Ø2.75 mm platform

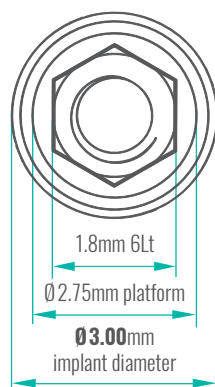

The BIOLEVEL implant with Ø3.0 diameter and Ø2.75 mm platform is exceptionally suitable for thinner than average bone structures for holding the toothworks on the long run.

The raw material of it is homogeneous, high solidity alloyed titanium.

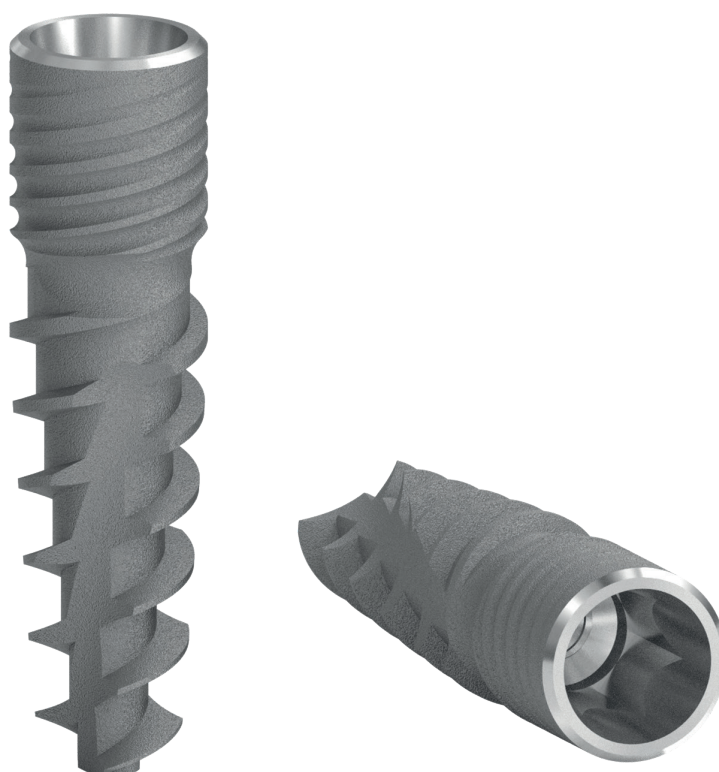

BIOLEVEL MANUAL IMPLANT KEY DRIVER



6Lt 1.8 mm
L 6 mm



6Lt 1.8 mm
L 12 mm



6Lt 1.8 mm
L 18 mm



BIOLEVEL MECHANICAL IMPLANT KEY DRIVER



6Lt 1.8 mm
L 6 mm



6Lt 1.8 mm
L 12 mm




6Lt 1.8 mm
L 18 mm



Sizes available of the **BIOLEVEL** implant with Ø2.75mm platform


Ø3.0

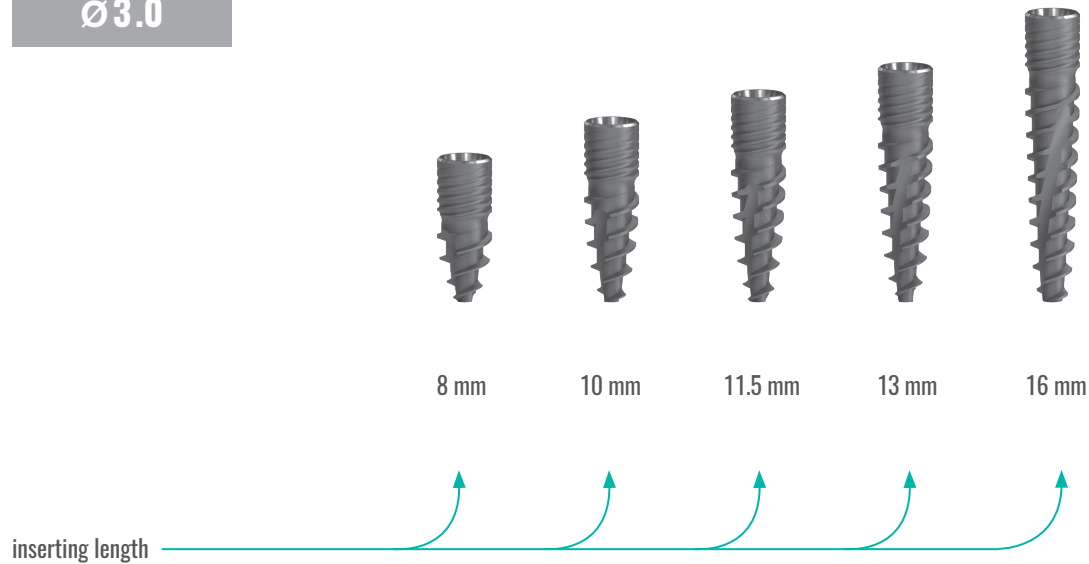


The drilling protocol of the **BIOLEVEL** implant with Ø2.75mm platform

Drilling Indicators:

- alternatively used
- ½ length drilling alternatively
- recommended drilling in ¾ or in full length

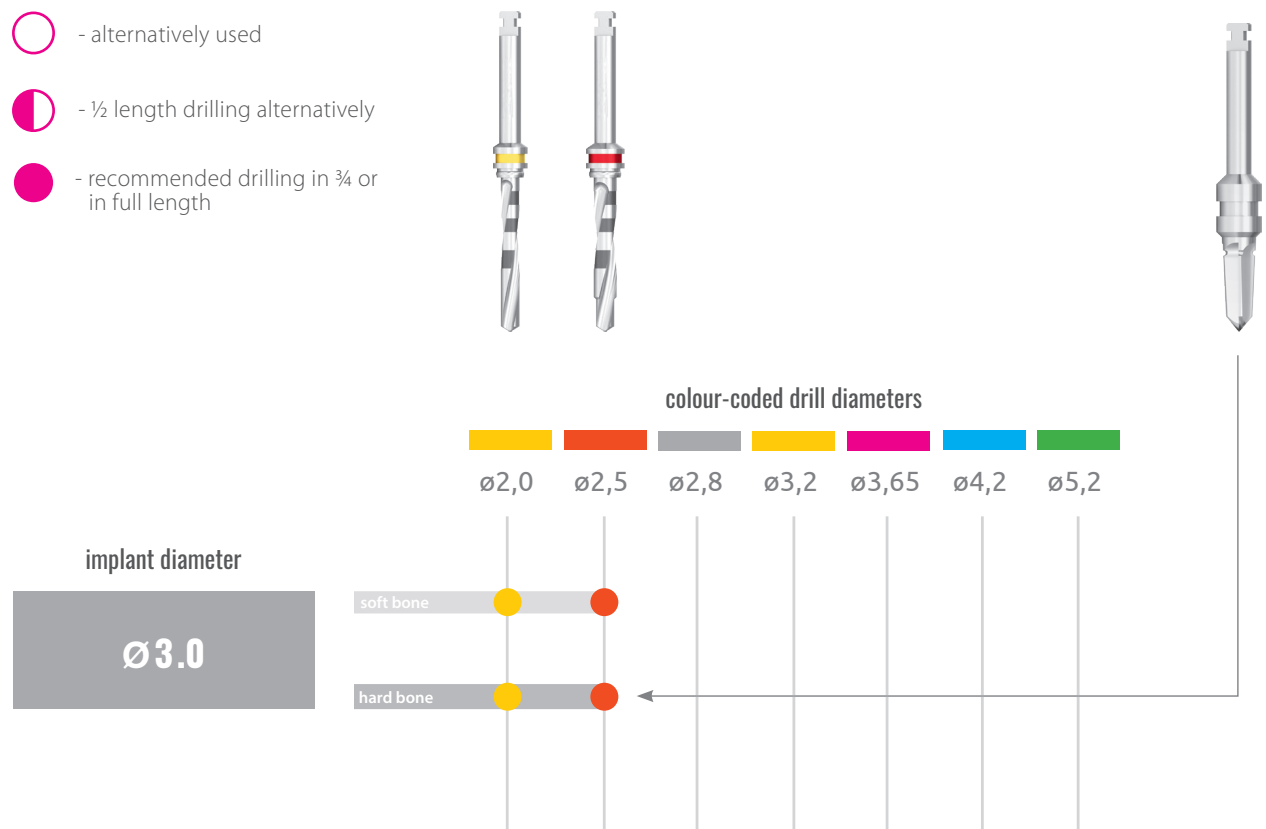


BIOLEVEL implants with Ø3.0 mm platform

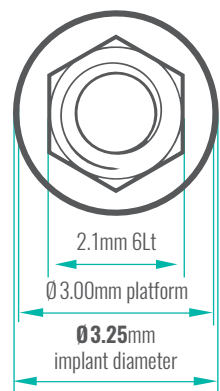


The BIOLEVEL implant with ø3.25 diameter and ø3.0 mm platform is exceptionally suitable for thinner than average bone structures for holding the toothworks on the long run.


The raw material of it is homogeneous, high solidity alloyed titanium.

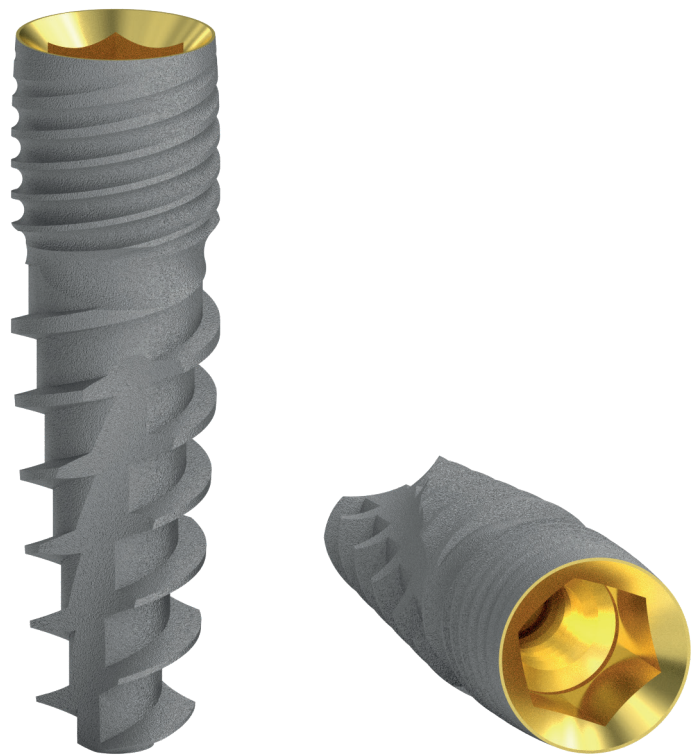

BIOLEVEL MANUAL IMPLANT KEY DRIVER

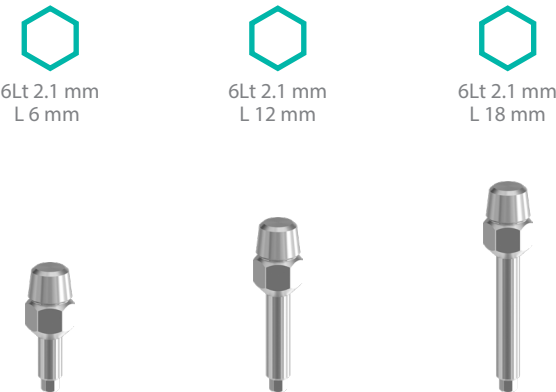


BIOLEVEL MECHANICAL IMPLANT KEY DRIVER

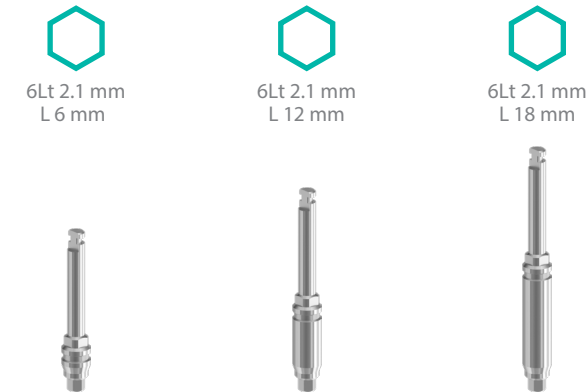

Sizes available of the **BIOLEVEL** implant with Ø3.0 mm platform


Ø3.25

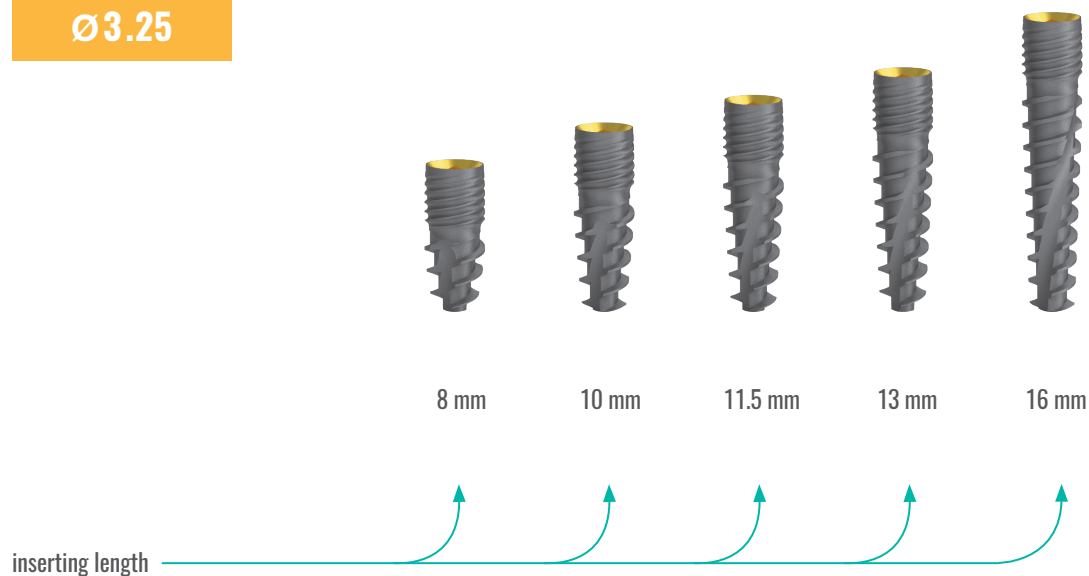


The drilling protocol of the **BIOLEVEL** implant with Ø3.0 mm platform

Drilling Indicators:


- - alternatively used
- ◐ - ½ length drilling alternatively
- - recommended drilling in ¾ or in full length

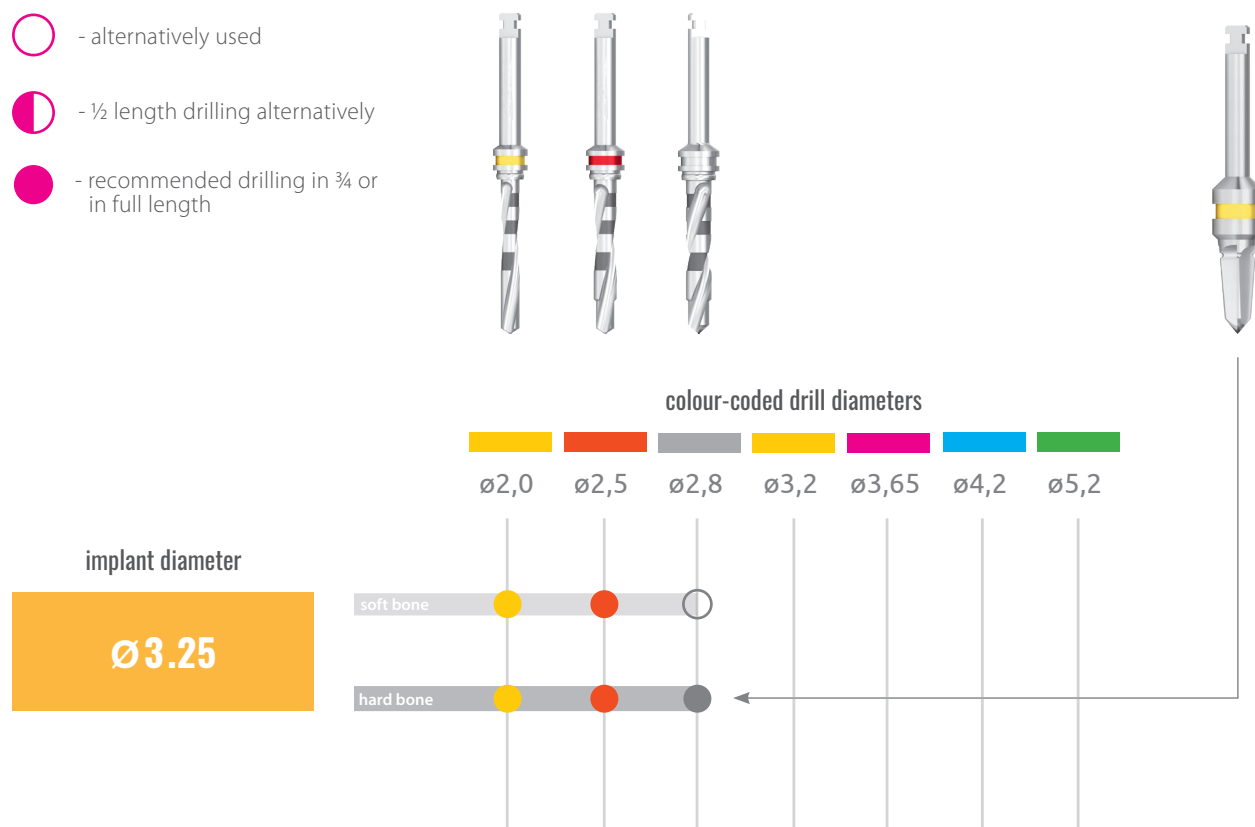

BIOLEVEL implants with Ø3.5 mm platform

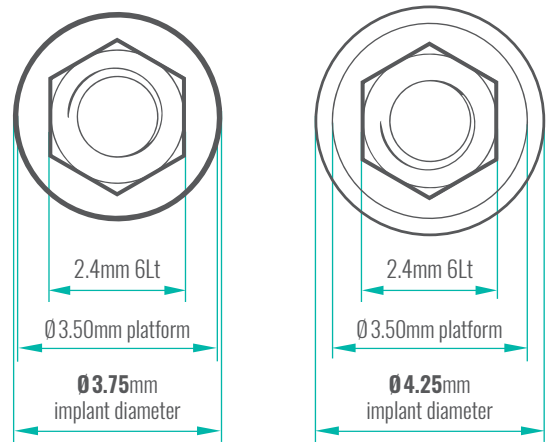

The BIOLEVEL implant with ø3.75 diameter and ø4.25 mm platform is exceptionally suitable for average bone structures for holding the toothworks on the long run. The 75 % of the occurring cases can be covered with this type.

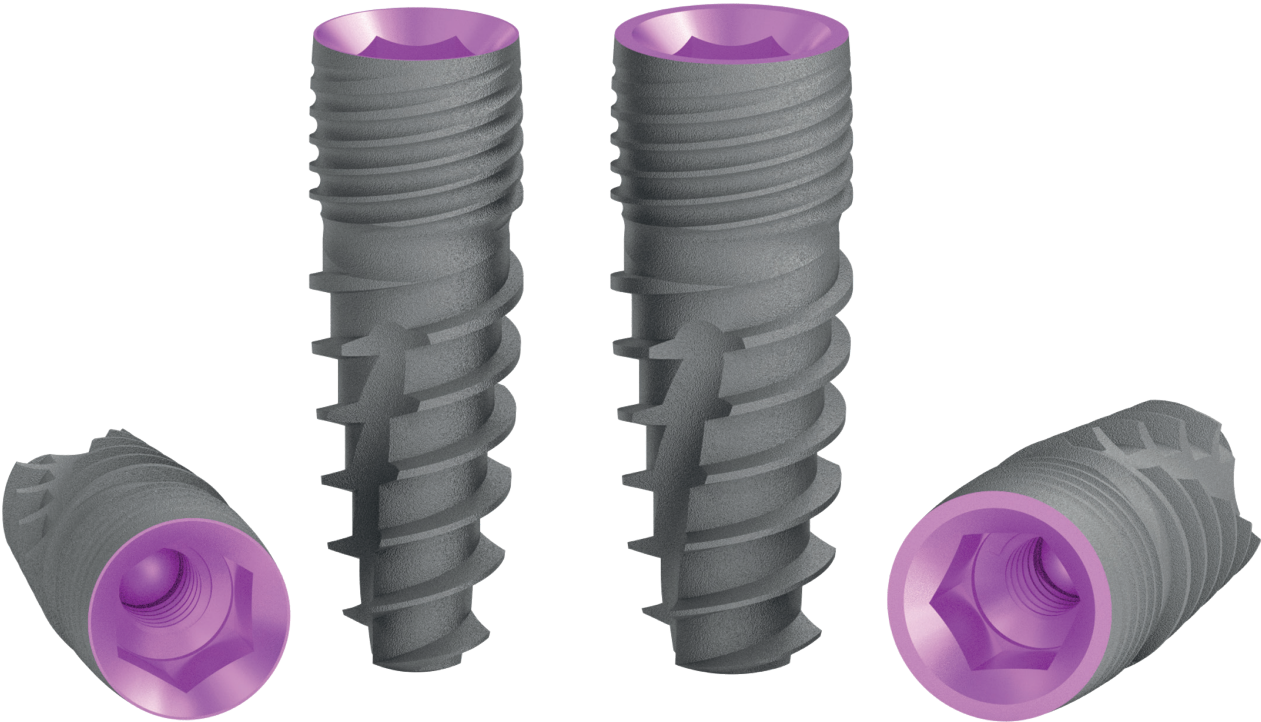

BIOLEVEL MANUAL IMPLANT KEY DRIVER




BIOLEVEL MECHANICAL IMPLANT KEY DRIVER




Sizes available of the **BIOLEVEL** implant with Ø3.5 mm platform

Ø3.75

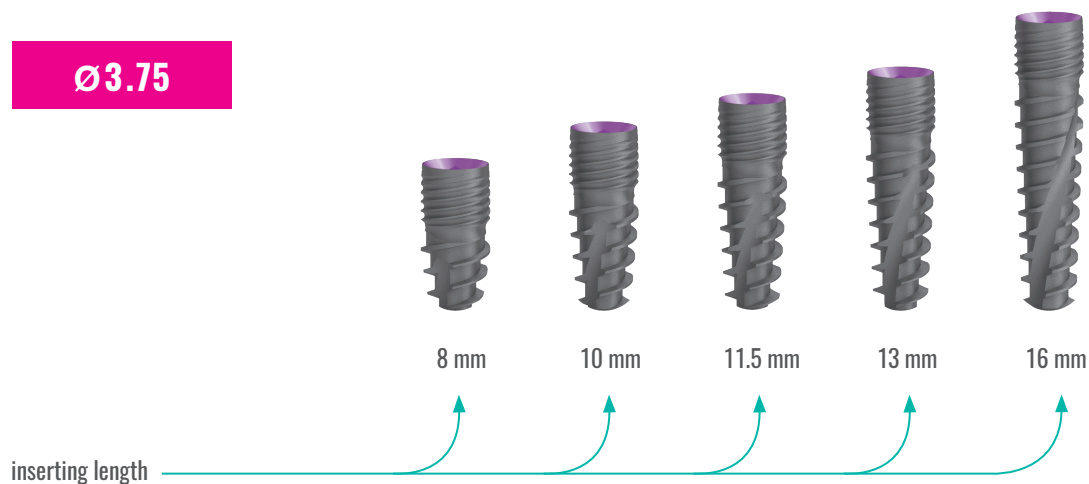

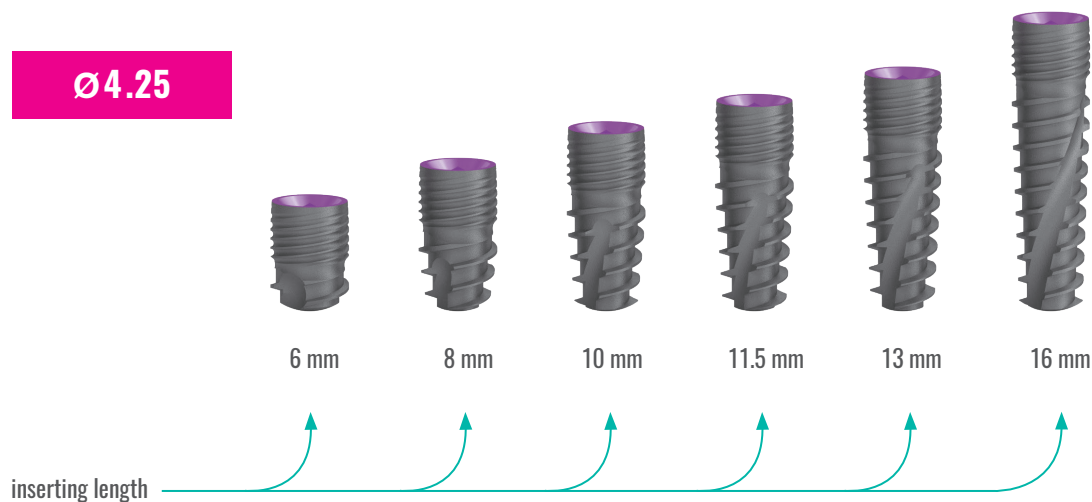


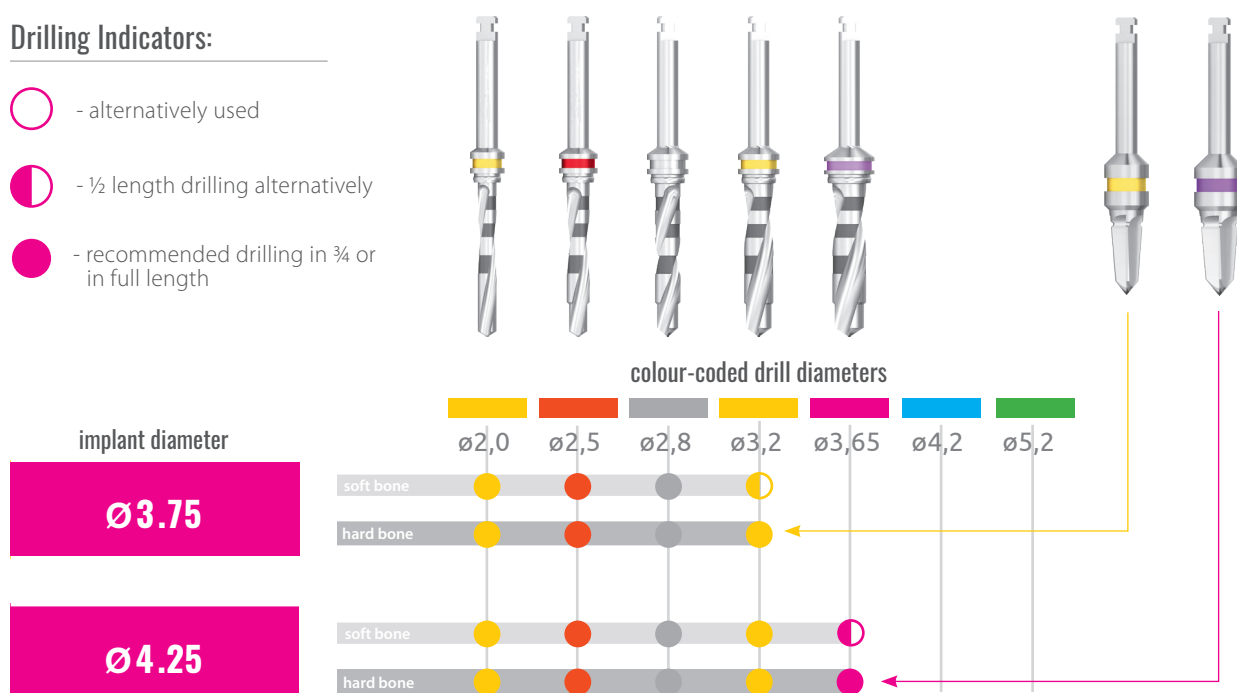
Ø4.25




The drilling protocol of the **BIOLEVEL** implant with Ø3.5 mm platform

Drilling Indicators:

-  - alternatively used
-  - ½ length drilling alternatively
-  - recommended drilling in ¾ or in full length




BIOLEVEL implants with Ø4.5 mm platform

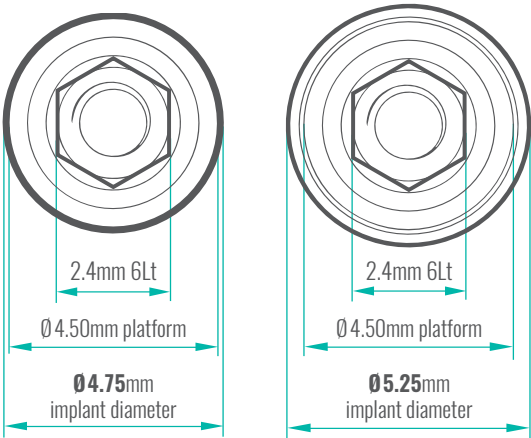


The thick BIOLEVEL implant with Ø4.50 and Ø5.25 diameters and Ø4.50 mm platform is exceptionally suitable for bigger than average bone supply and normal chewing ability for holding the toothworks on the long run.

The raw material of it is homogeneous, high solidity alloyed titanium.

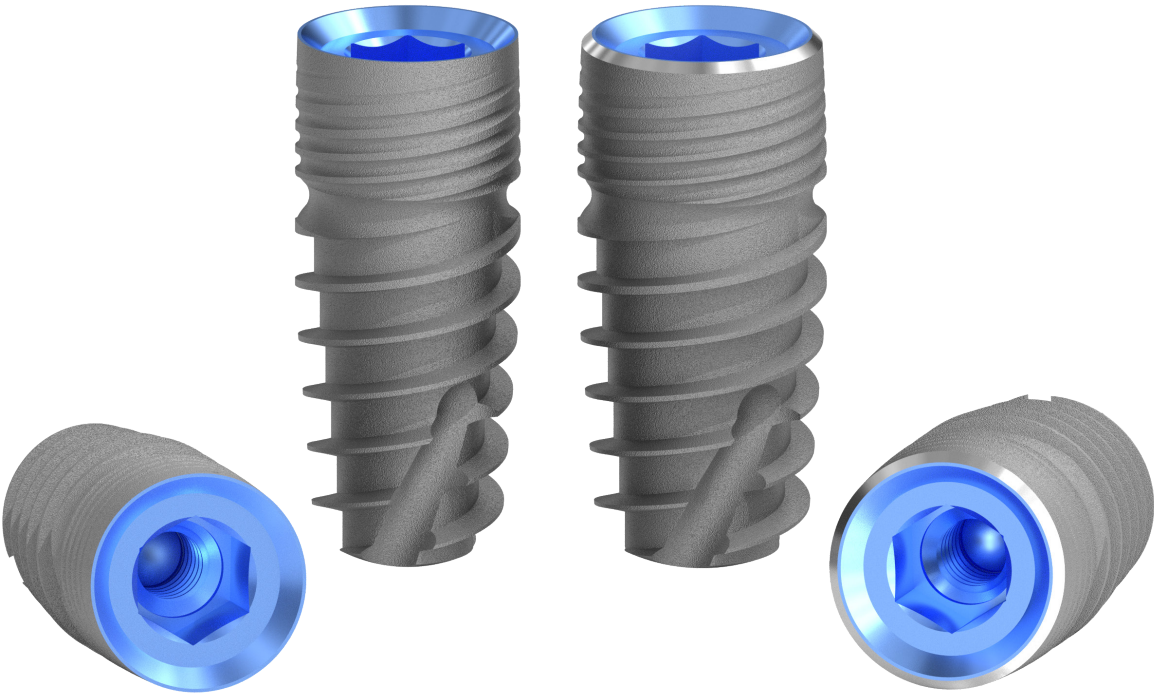

BIOLEVEL MANUAL IMPLANT KEY DRIVER

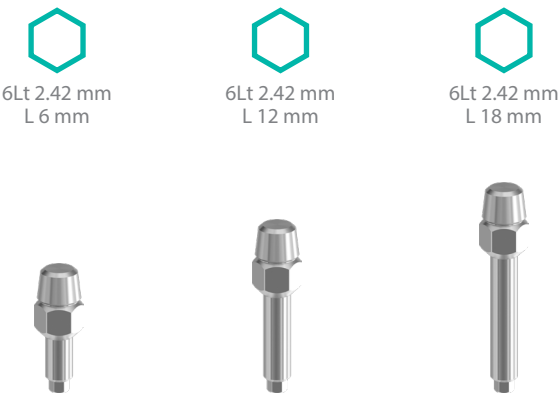


BIOLEVEL MECHANICAL IMPLANT KEY DRIVER




Sizes available of the **BIOLEVEL** implant with Ø4.5 mm platform

Ø4.75

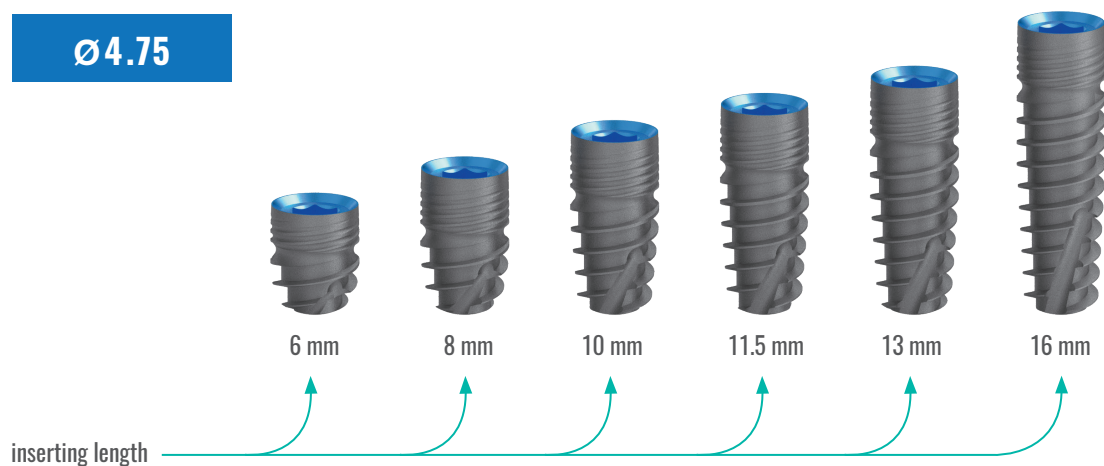

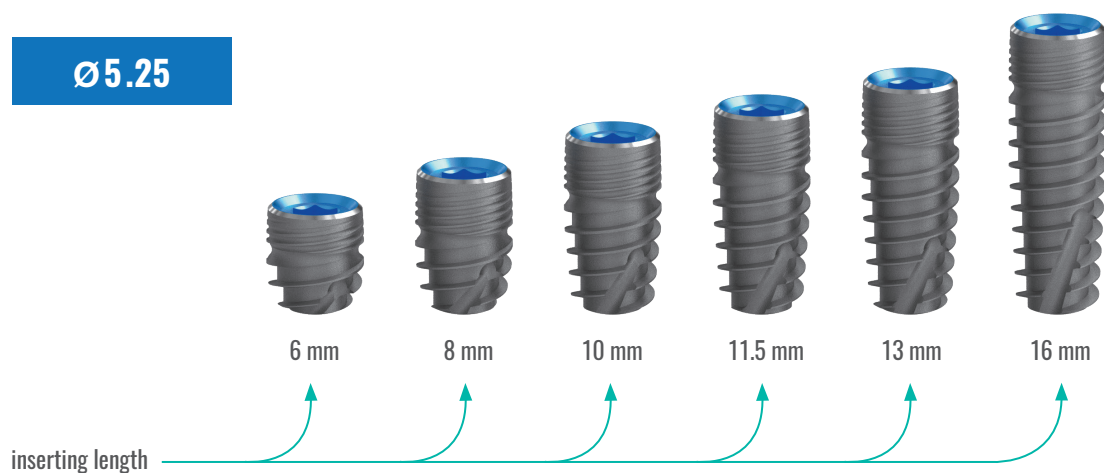


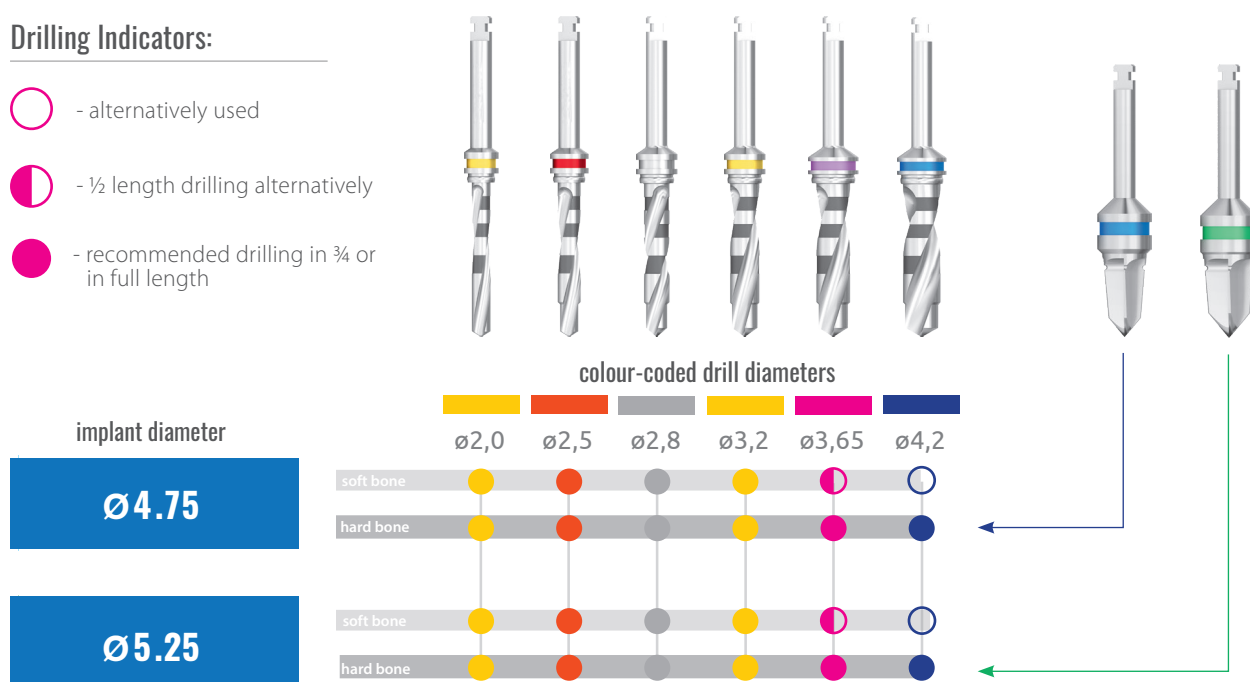
Ø5.25




The drilling protocol of the **BIOLEVEL** implant with Ø4.5 mm platform

Drilling Indicators:

-  - alternatively used
-  - ½ length drilling alternatively
-  - recommended drilling in ¾ or in full length




BIOLEVEL implants with Ø5.7 mm platform

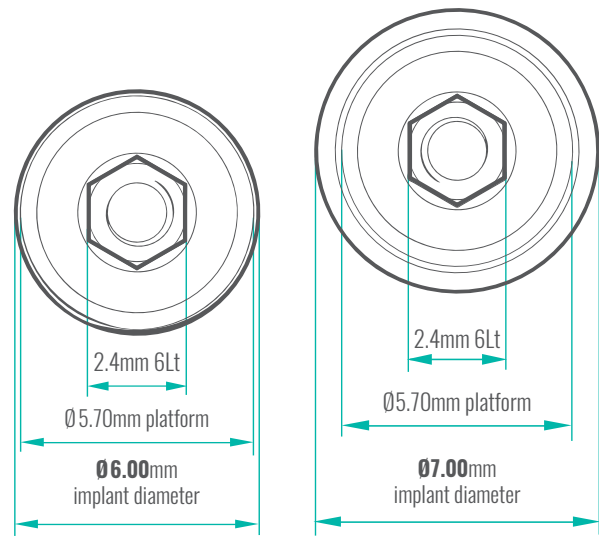

The thick BIOLEVEL implant with Ø6,00 and Ø 7,00 diameters and Ø5,7 mm platform is exceptionally suitable for average bone structures for holding the toothworks on the long run. The 75 % of the occurring cases can be covered with this type.

The raw material of it is homogeneous, high solidity alloyed titanium.

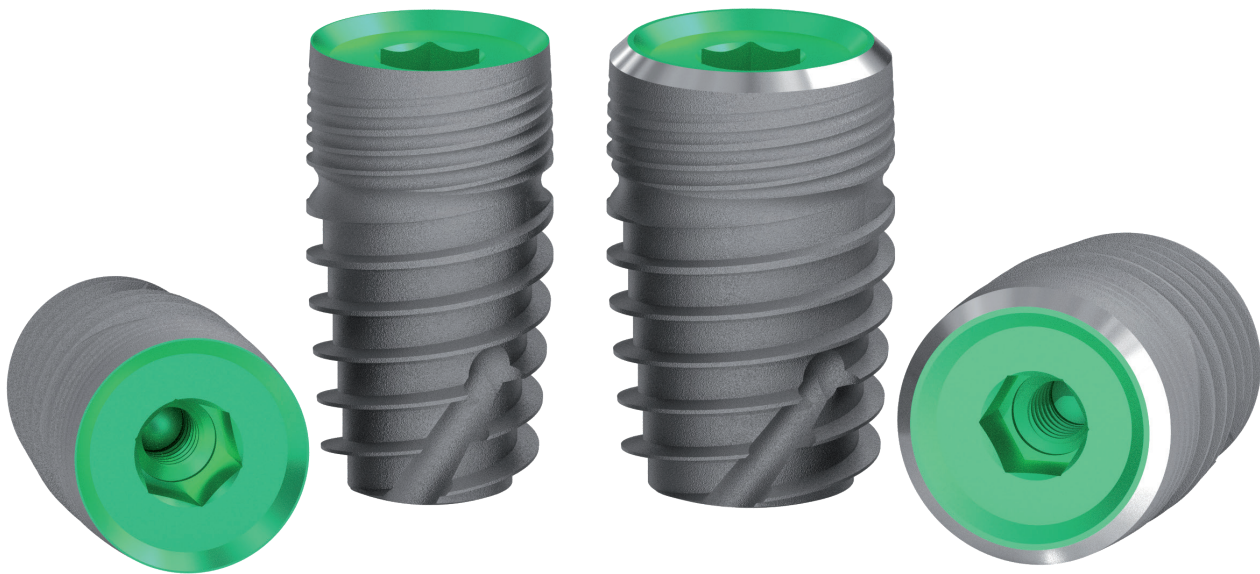

BIOLEVEL MANUAL IMPLANT KEY DRIVER



6Lt 2.42 mm
L 6 mm



6Lt 2.42 mm
L 12 mm



6Lt 2.42 mm
L 18 mm



BIOLEVEL MECHANICAL IMPLANT KEY DRIVER



6Lt 2.42 mm
L 6 mm





6Lt 2.42 mm
L 12 mm



6Lt 2.42 mm
L 18 mm



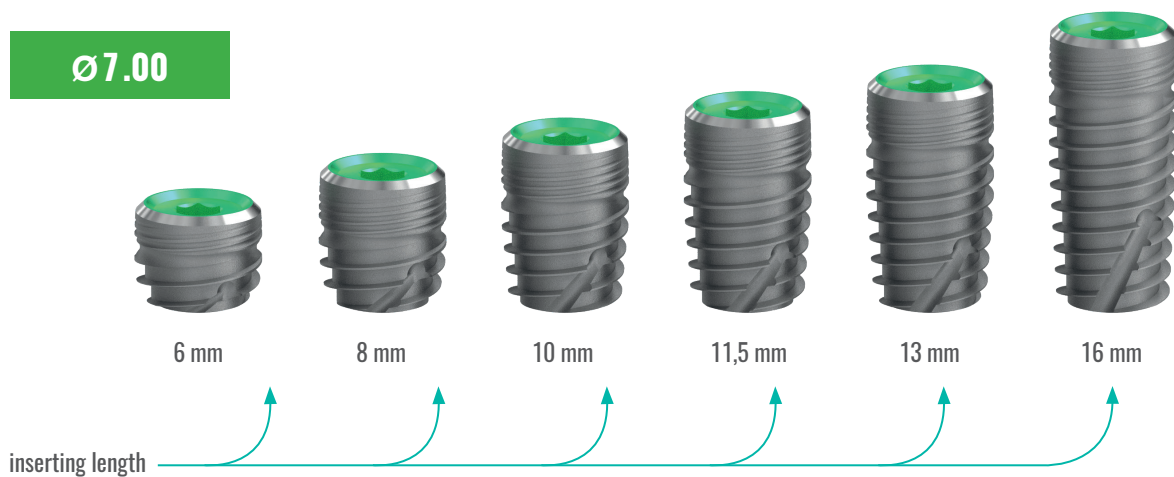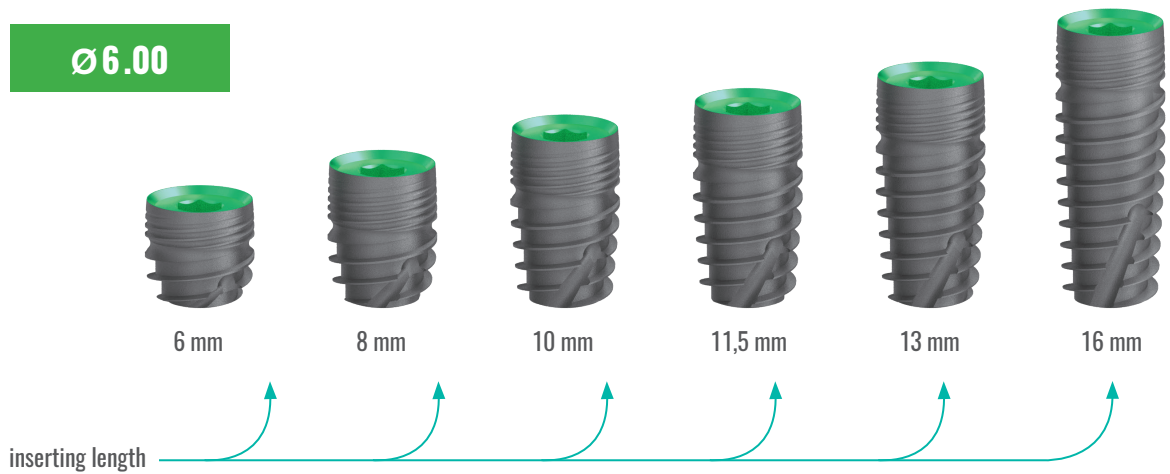


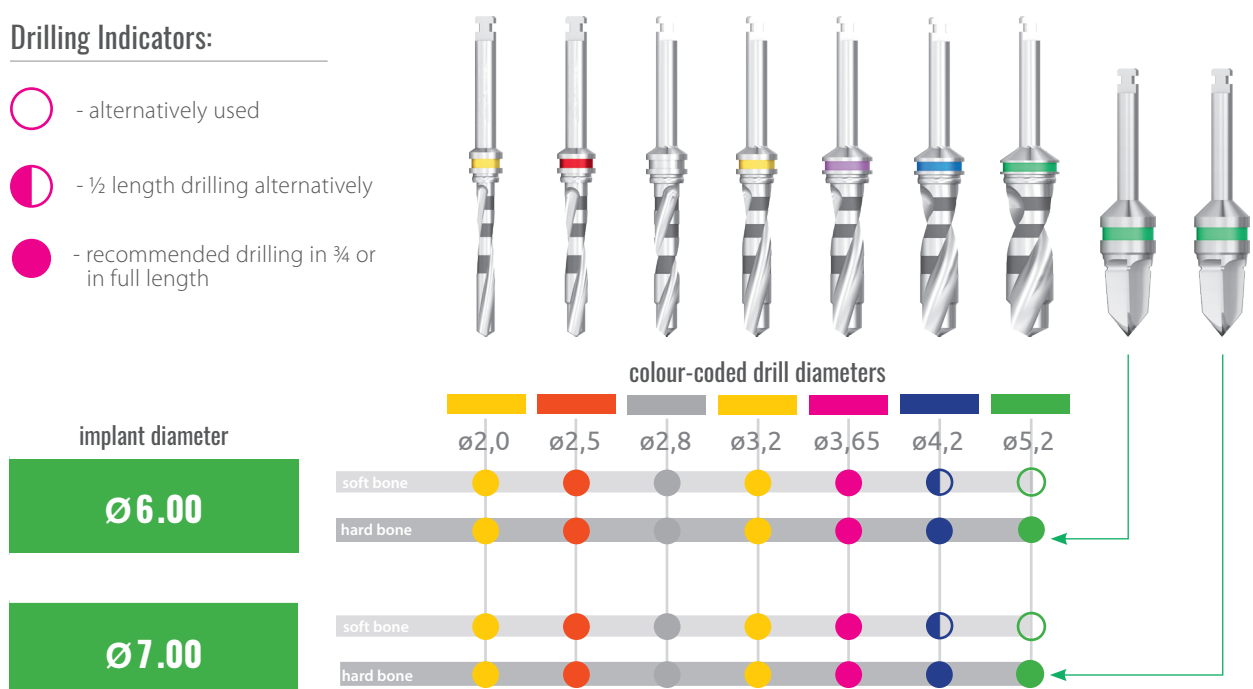
Sizes available of the **BIOLEVEL** implant with Ø5.7 mm platform



The drilling protocol of the **BIOLEVEL** implant with Ø5.7 mm platform

Drilling Indicators:

-  - alternatively used
-  - ½ length drilling alternatively
-  - recommended drilling in ¾ or in full length






BIOLEVEL
Abutment system



ABUTMENT SYSTEM | TABLE OF CONTENTS

BIOLEVEL abutments	30
Sizes available of BIOLEVEL abutments	32
Accessories of abutments	36

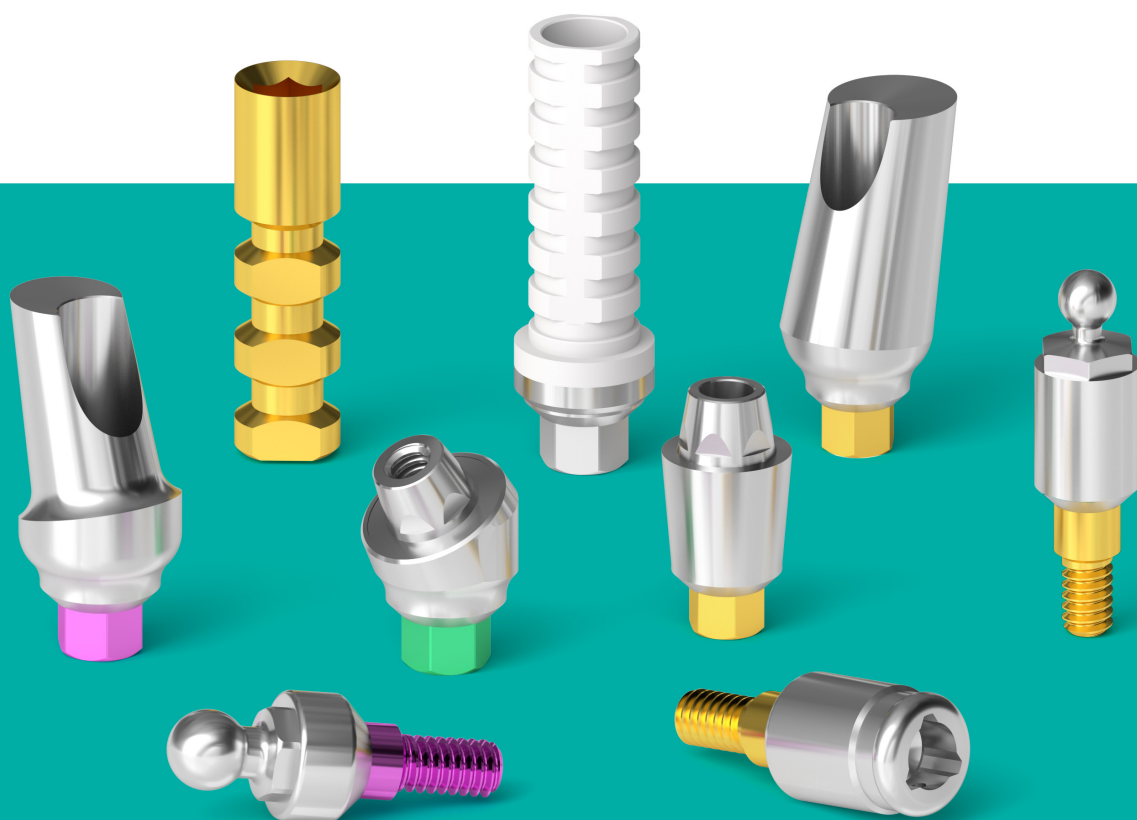

BIOLEVEL abutments

1. Implants

PROSTHETIC ELEMENTS


- 2. Technical implant
- 3. Healing cap, narrow
- 4. Healing cap, anatomical
- 5. Sampling head for closed spoon
- 6. Sampling head for open spoon
- 7. Temporary head, through-bolted, positioned
- 8. Temporary head, through-bolted, non-positioned
- 9. Temporary head, through-bolted, positioned, PEEK
- 10. Temporary head, through-bolted, non-positioned, PEEK

FOR GLUABLE TOOTHWORK

- 11. Narrow head, straight
- 12. Narrow head oblique
- 13. Universal head, straight
- 14. Universal head, oblique
- 15. Anatomical head, straight
- 16. Anatomical head, oblique
- 17. Trapezoidal head
- 18. Delta head

IMPLANT- LEVEL CASTING HEADS

- 19. Castable plastic head, positioned
- 20. Castable plastic head, non-positioned

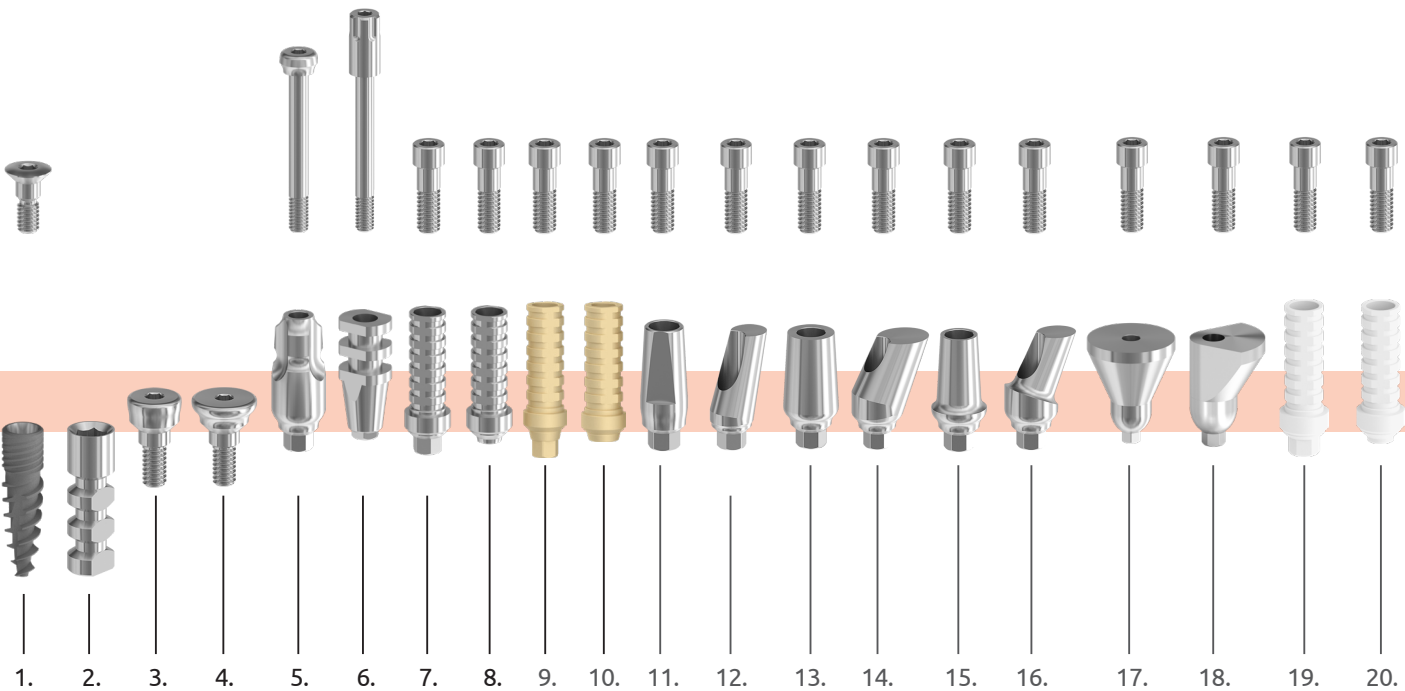

21. Cobalt chromium-based casting head, positioned
22. Cobalt chromium-based casting head, non-positioned
23. Interface, positioned
24. Interface, non-positioned

FOR REMOVABLE TOOTHWORK

25. Ball-head
26. Locator head, straight


FOR SCREWED TOOTHWORK

27. Multi-unit head, straight
28. Multi-unit head, through-bolted
29. Multi-unit head, oblique


30. MC head, oblique
31. Multi-unit SR head, screwable
32. Multi-unit SR head, through-bolted with threaded head
33. Multi-unit SR head, oblique

ELEMENTS OF CAD-CAM SYSTEM


34. Titanium base
35. Press ceramic base
36. Tube-head, positioned
37. Tube-head, non-positioned
38. Scanbody head, through-bolted
39. Scanbody head, screwable

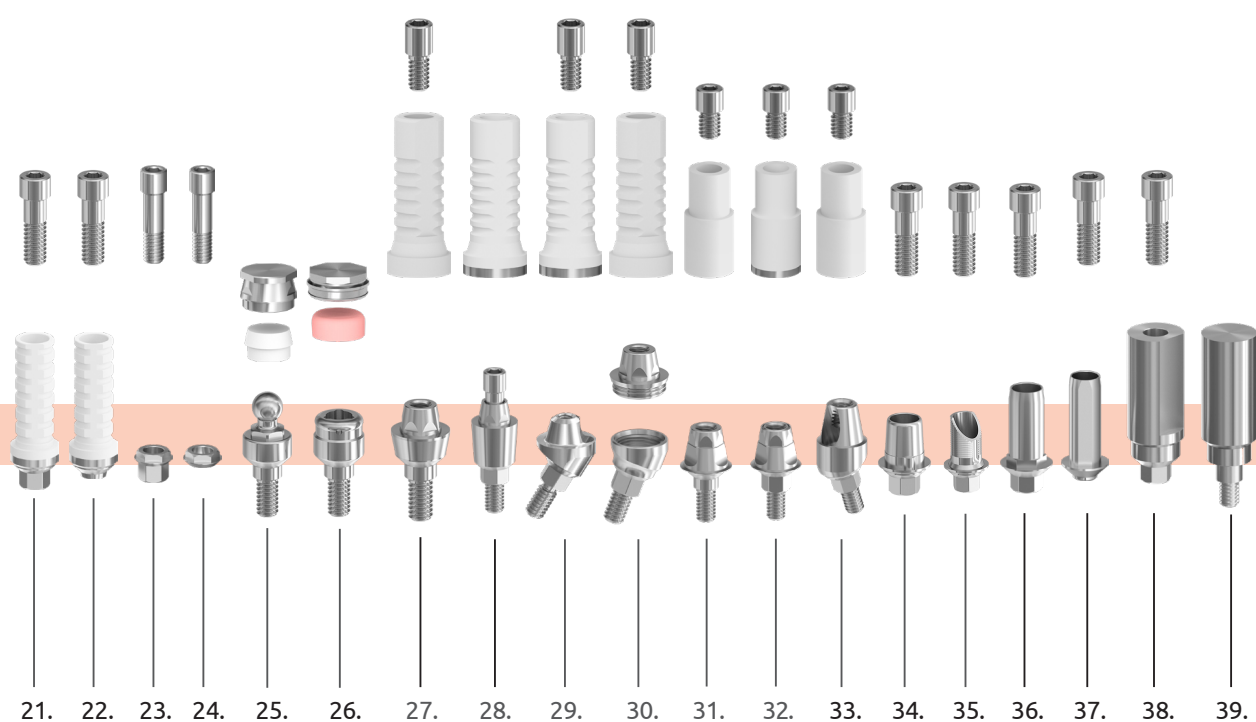


The selections of **BIOLEVEL** abutments

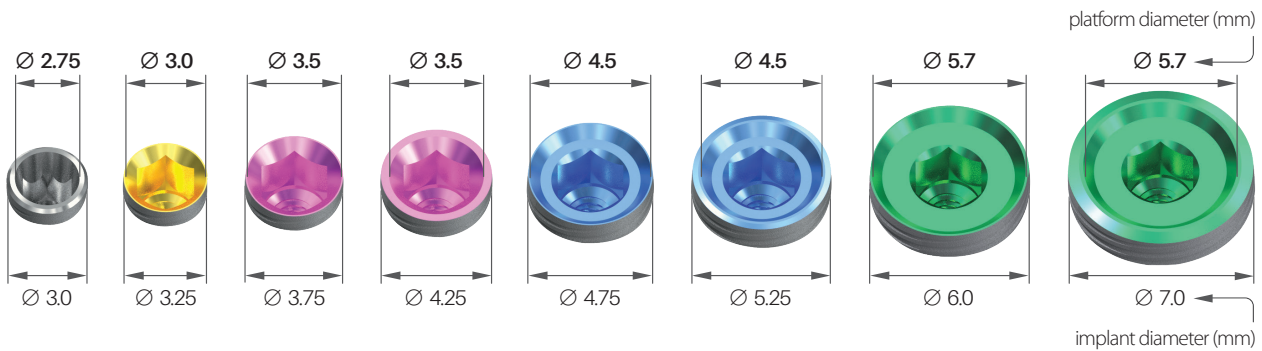


TECHNICAL IMPLANT

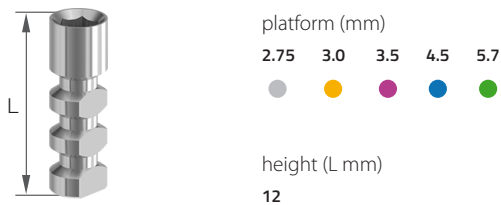


SAMPLING HEAD FOR OPEN SPOON

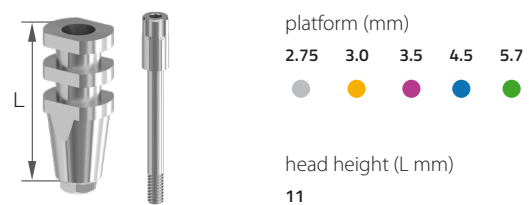


HEALING CAP, NARROW

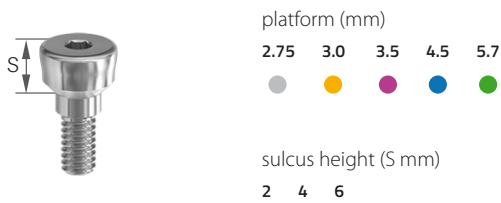


TEMPORARY HEAD, THROUGH-BOLTED, POSITIONED

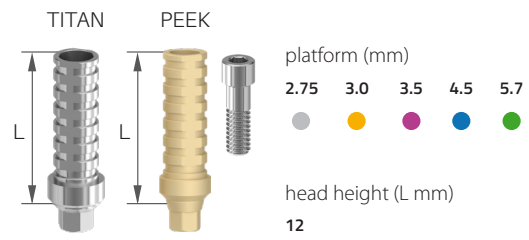


HEALING CAP, ANATOMICAL

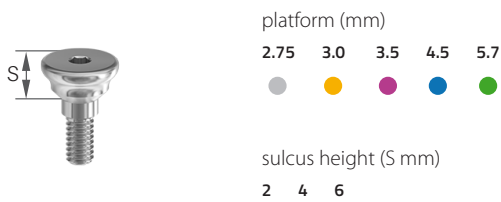


TEMPORARY HEAD, THROUGH-BOLTED, NON-POSITIONED

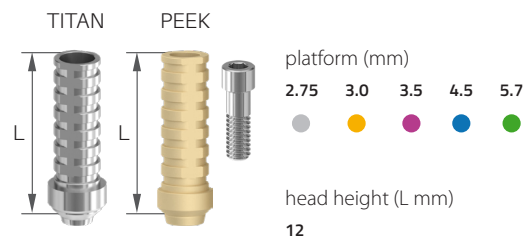


SAMPLING HEAD FOR CLOSED SPOON

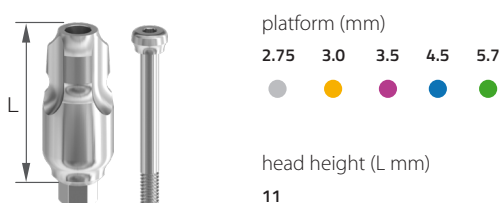


NARROW HEAD, STRAIGHT

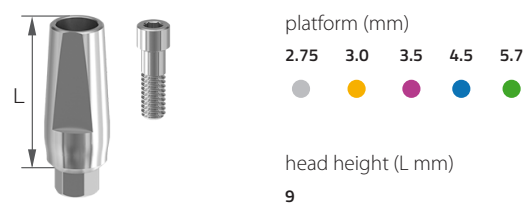


NARROW HEAD, OBLIQUE 15°, 25°

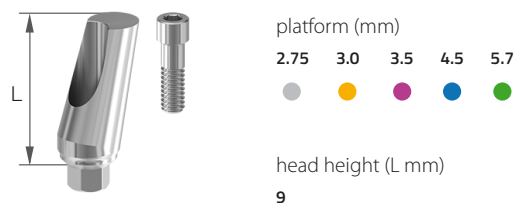


TRAPEZOIDAL HEAD 15°, 25°, 35°, 45°

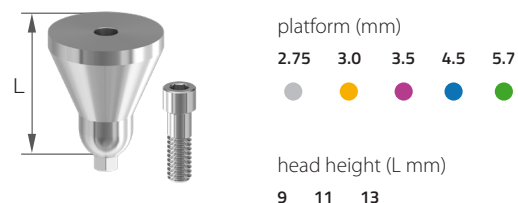


UNIVERSAL HEAD, STRAIGHT

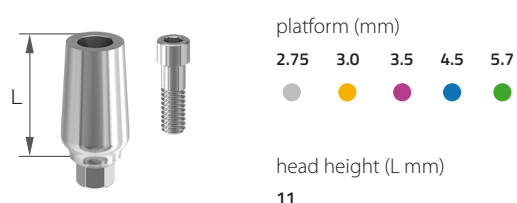


DELTA HEAD 15°, 25°, 35°, 45°

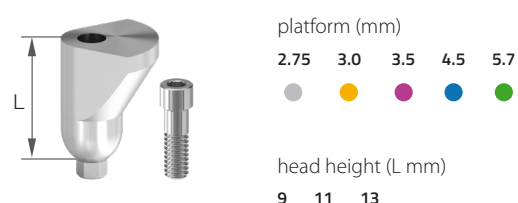


UNIVERSAL HEAD, OBLIQUE 15°, 25°, 35°, 45°

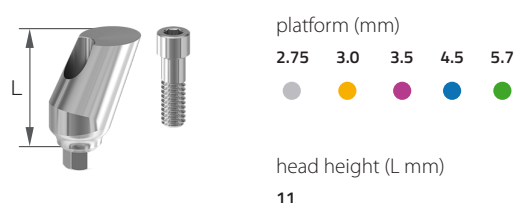


CASTABLE PLASTIC HEAD, POSITIONED

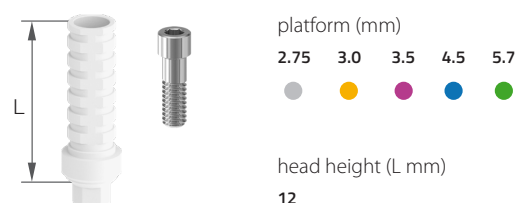


ANATOMICAL HEAD, STRAIGHT

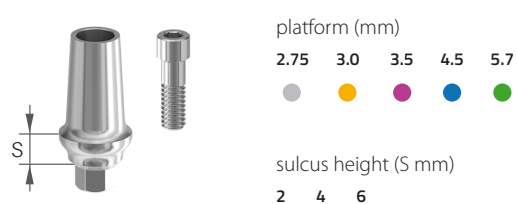


CASTABLE PLASTIC HEAD, NON-POSITIONED

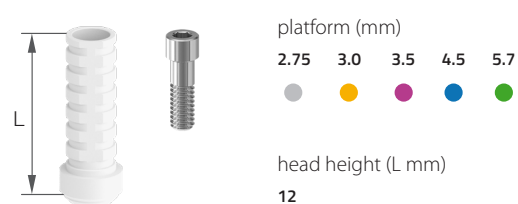

ANATOMICAL HEAD, OBLIQUE 15°, 25°

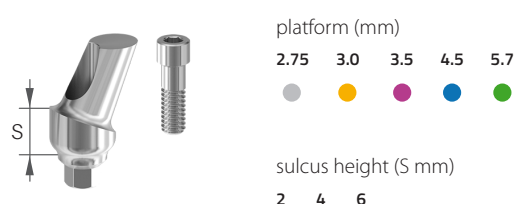


CO-CR, METAL BASED CASTING HEAD, POSITIONED

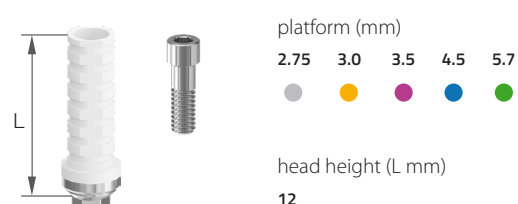


The selections of BIOLEVEL abutments


CO-CR, METAL BASED CASTING HEAD , NON-POSITIONED

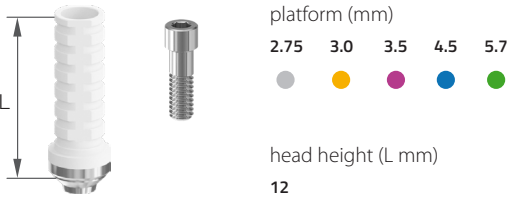


MULTI-UNIT HEAD, STRAIGHT

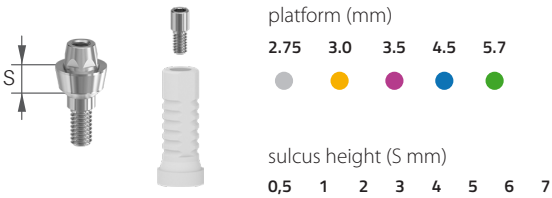


BR INTERFACE, POSITIONED

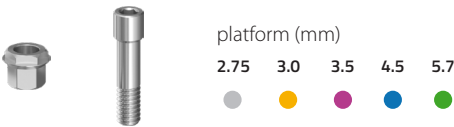


MULTI-UNIT HEAD, THROUGH-BOLTED

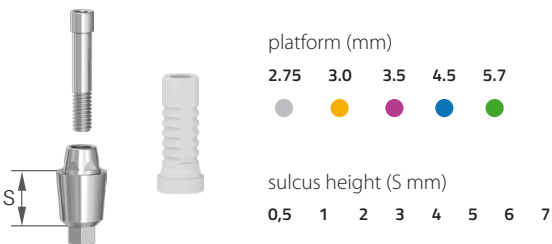


BR INTERFACE, NON-POSITIONED

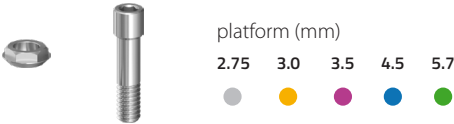


MULTI-UNIT OBLIQUE HEAD, 20°, 30°

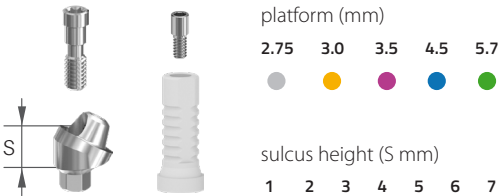


BALL-HEAD

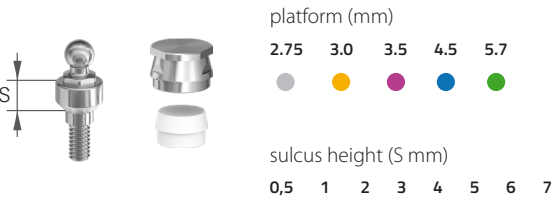


MC OBLIQUE HEAD, 20°, 30°

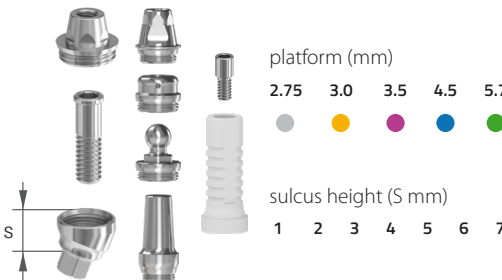


LOCATOR HEAD

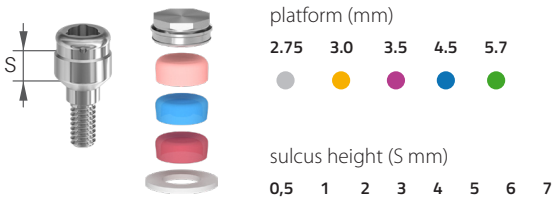


MULTI-UNIT SR HEAD, SCREWABLE

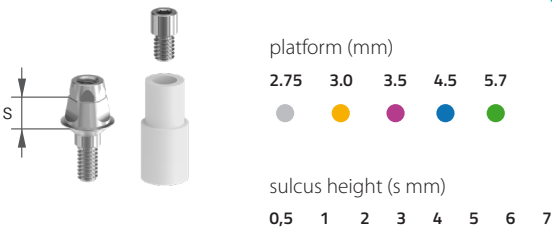


MULTI-UNIT SR HEAD THROUGH-BOLTED

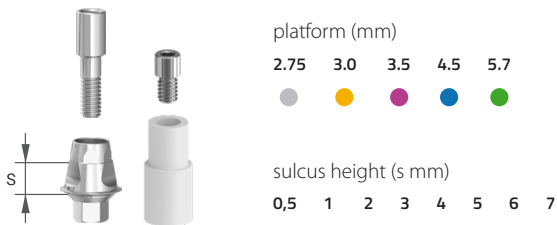


TUBE HEAD, POSITIONED

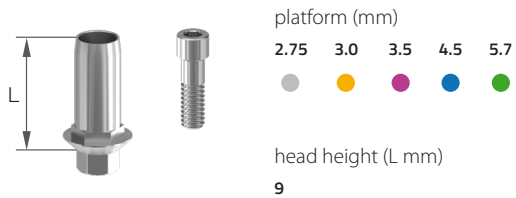


MULTI-UNIT SR HEAD, OBLIQUE 20°, 30°

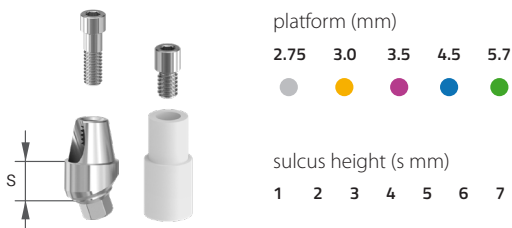


TUBE HEAD, NON-POSITIONED

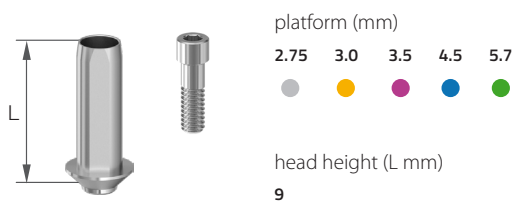


TITANIUM BASE

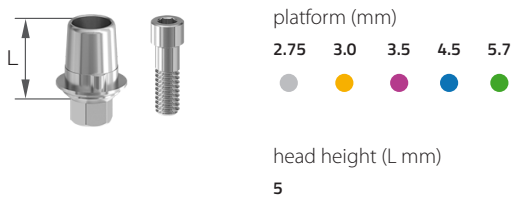


SCANBODY HEAD, THROUGH-BOLTED

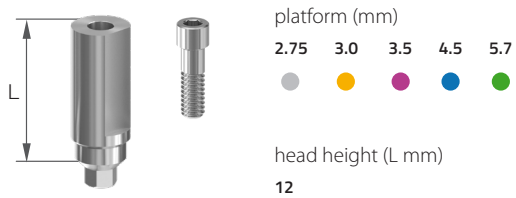

PRESS CERAMIC BEASE

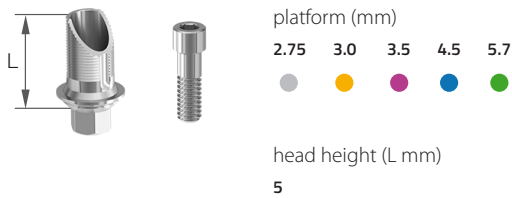

SCANBODY HEAD, SCREWABLE

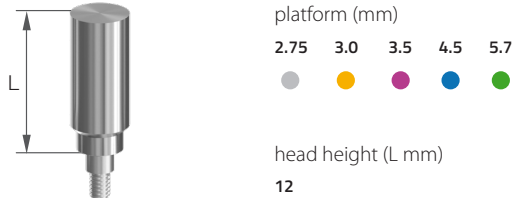

Abutment accessories and screws of BIOLEVEL

HEAD SCREW, SURGICAL



platform (mm)

2.75	3.0	3.5	4.5	5.7

MULTI-UNIT THROUGH-BOLT



platform (mm)

2.75	3.0	3.5	4.5	5.7

SAMPLING HEAD SCREW, FOR CLOSED SPOON



platform (mm)

2.75	3.0	3.5	4.5	5.7

SR-HEAD SCREW



platform (mm)

2.75	3.0	3.5	4.5	5.7

It is the same in every diameter.

SAMPLING HEAD SCREW, FOR OPEN SPOON



platform (mm)

2.75	3.0	3.5	4.5	5.7

SR-THROUGH-BOLT



platform (mm)

2.75	3.0	3.5	4.5	5.7

MULTI-UNIT HEAD SCREW



platform (mm)

2.75	3.0	3.5	4.5	5.7

It is the same in every diameter.

Abutment accessories and screws of BIOLEVEL

BALL HEAD CAP, NORMAL



platform (mm)
2.75 3.0 3.5 4.5 5.7
sphere diameter 2,5 mm

CASTABLE HEAD FOR MULTI-UNIT HEAD, Co-Cr, METAL BASED



platform (mm)
2.75 3.0 3.5 4.5 5.7
It is the same in every diameter.

BALL HEAD CAP, MICRO



platform (mm)
2.75 3.0 3.5 4.5 5.7
sphere diameter 1,8 mm

CASTABLE HEAD FOR SR HEAD



platform (mm)
2.75 3.0 3.5 4.5 5.7
It is the same in every diameter.

LOCATOR HEAD CAP SET



pink cap:
10-20° deviations, 3lbs retention
blue cap:
10-20° deviations, 1,5lbs retention
red cap:
20-40° deviations, 1lbs retention
It is the same in every diameter.

CASTABLE HEAD FOR SR HEAD, Co-Cr, METAL BASED



platform (mm)
2.75 3.0 3.5 4.5 5.7
It is the same in every diameter.


CASTABLE HEAD FOR MULTI-UNIT HEAD



platform (mm)
2.75 3.0 3.5 4.5 5.7
It is the same in every diameter.



BIOLEVEL
INSTRUMENT KITS

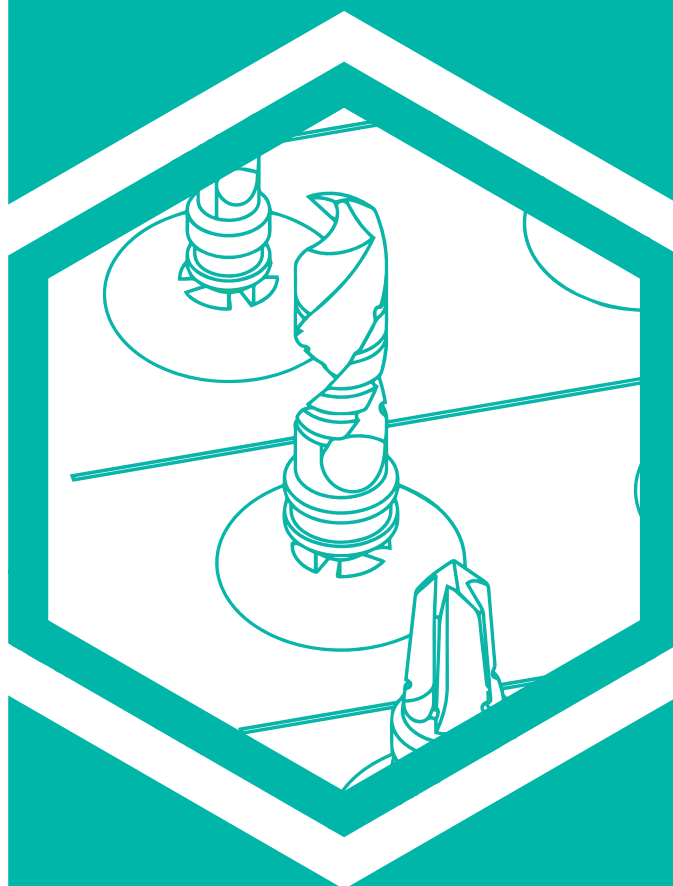

BIOLEVEL instrument kits


Our instrument kits consist of the inevitable instruments for dental implantation. The Large Instrument Kit includes 33 instruments, in a wide range of sizes in order to get versatile utilization.

The plate, which consists the instruments, is also suitable for sterilizing the instruments. The sterilizing can be done separately, as the plate can be uplifted from the box, or together with the box.

Large instrument kit




Small instrument kit

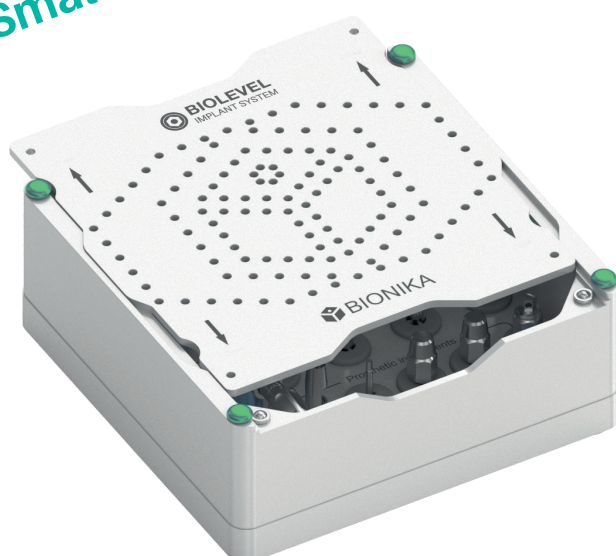

The instrument trays are built up according to the surgical technique order, labelling makes their use easier.

The Small Instrument Kit is a practical and more economical solution. They include the inevitable instruments for surgeries as in the large instrument kit, only in smaller range of sizes. The small instrument tray consists of 19 instruments.

The large instrument kit

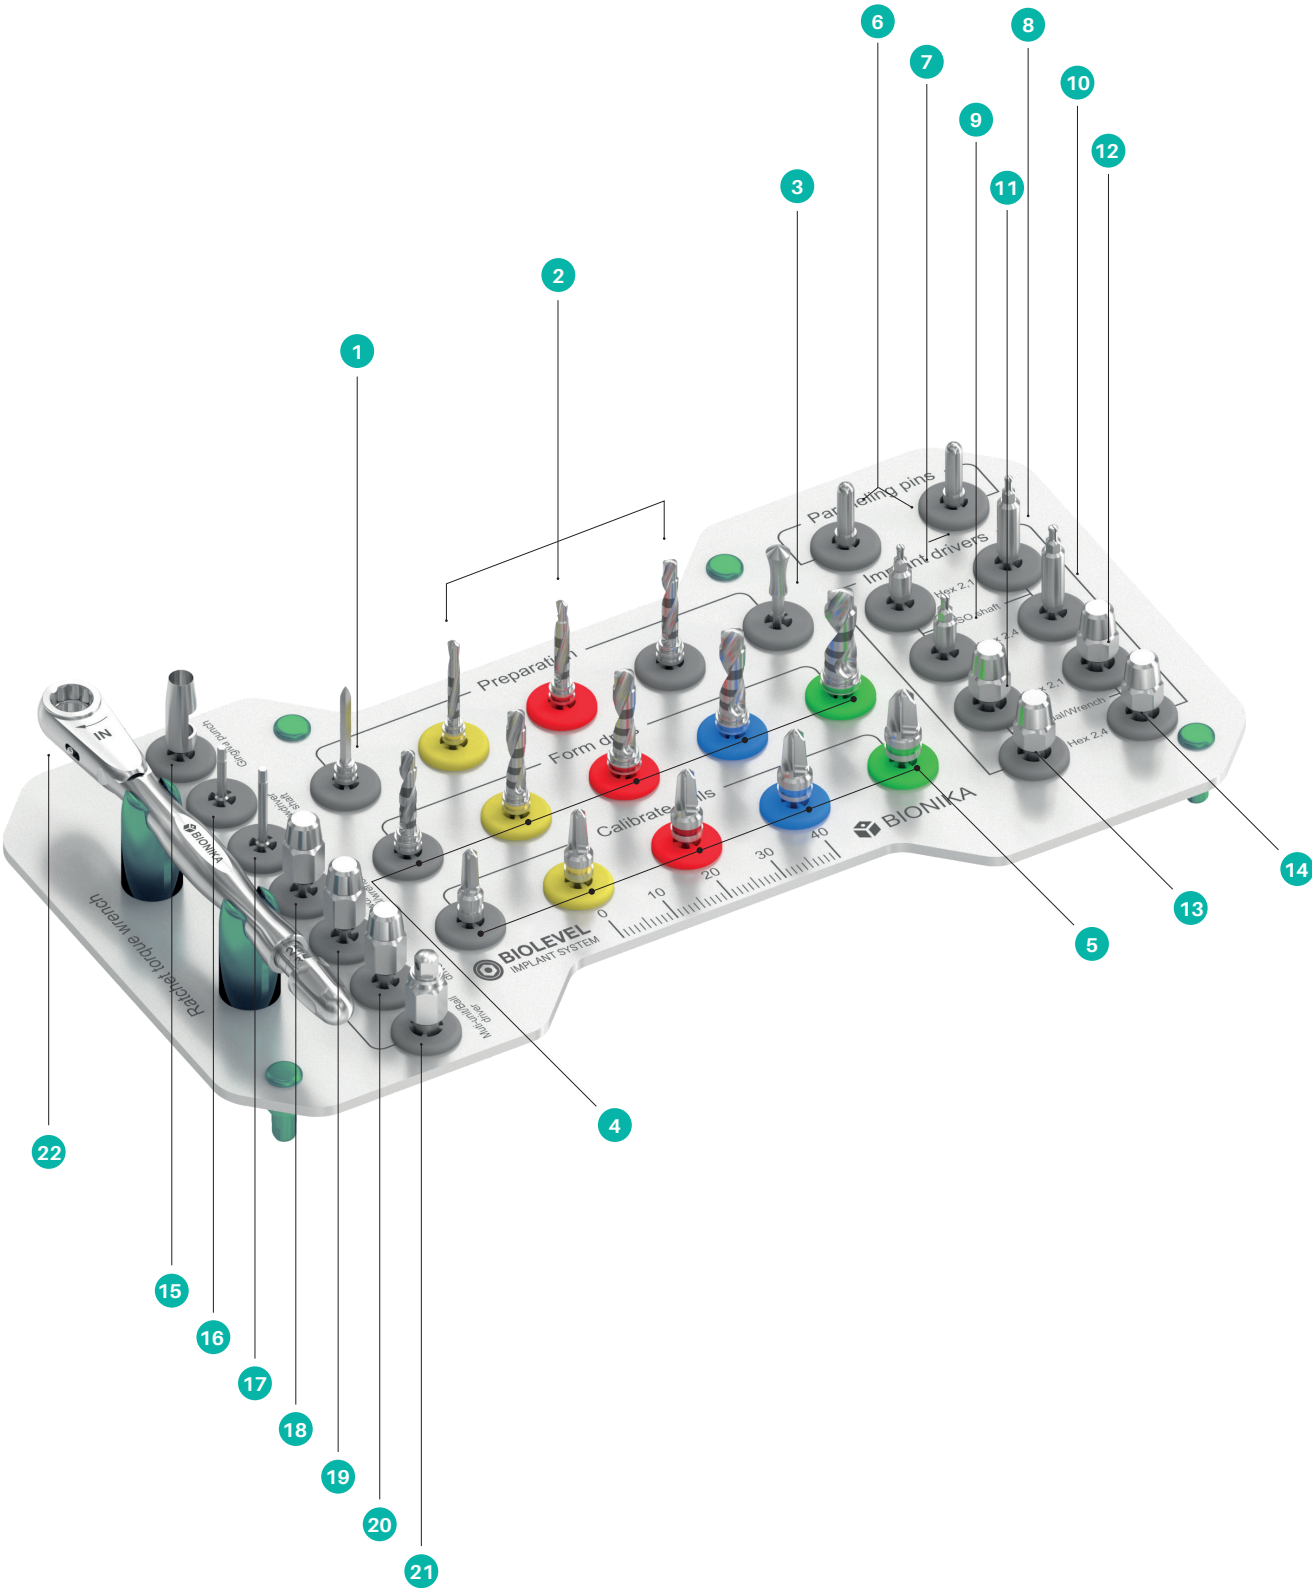

- 1 Spear-pointed drill ▼



- 2 Pre-drills ▼



- 3 Depth gauge ▼



- 4 Core drills ▼



- 5 Thread calibrator drills ▼



- 6 Indicators ▼



- 7 Implant driver, mechanical, 6Lt2, 1xL6 ▼



- 8 Implant driver, mechanical, 6Lt2, 1xL12 ▼



- 9 Implant driver, mechanical, 6Lt2, 4xL6 ▼



- 10 Implant driver, mechanical, 6Lt2, 4xL12 ▼



- 11 Implant driver, manual, 6Lt2, 1xL6 ▼



- 12 Implant driver, manual, 6Lt2, 1xL12 ▼



- 13 Implant driver, manual, 6Lt2, 4xL6 ▼



- 14 Implant driver, manual, 6Lt2, 4xL12 ▼



- 15 Gingiva punch Ø4,0xL15 ▼



- 16 Head wrench, mechanical 6Lt1, 27xL10 ▼



- 17 Head wrench, mechanical 6Lt1, 27xL15 ▼



- 18 Head wrench, manual 6Lt1, 27xL10 ▼



- 19 Head wrench, manual 6Lt1, 27xL15 ▼



- 20 Locator key ▼




- 21 Multi-unit/ball-head key, 6Lt2, 7 ▼



- 22 Ratchet torque wrench ▼



Small instrument kit

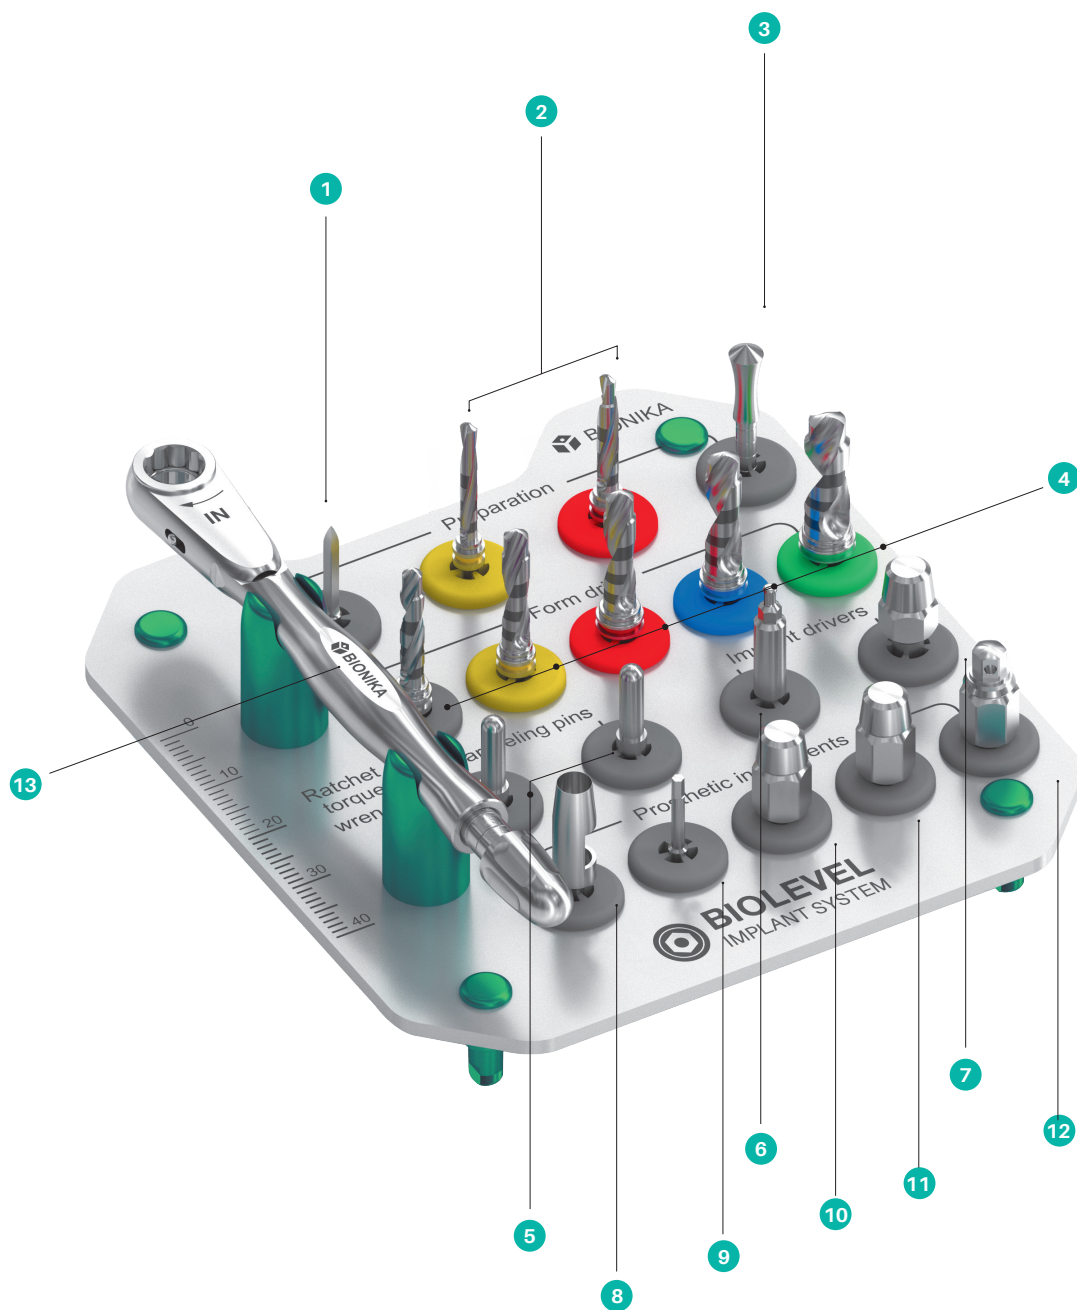

1 Spear-pointed drill ▼



2 Pre-drills ▼



3 Depth gauge ▼



4 Core drills ▼



5 Paralleling pins ▼



6 Implant driver, mechanical, 6Lt2,4xL12 ▼



7 Implant driver, manual, 6Lt2,4xL12 ▼



8 Gingiva punch Ø4,0xL15 ▼



9 Head wrench, mechanical 6Lt1,27xL10 ▼



10 Head wrench, manual 6Lt1,27xL10 ▼



11 Locator key ▼




12 Multi-unit/ball-head key, 6Lt2,7 ▼



13 Ratchet torque wrench ▼



Surgical drills

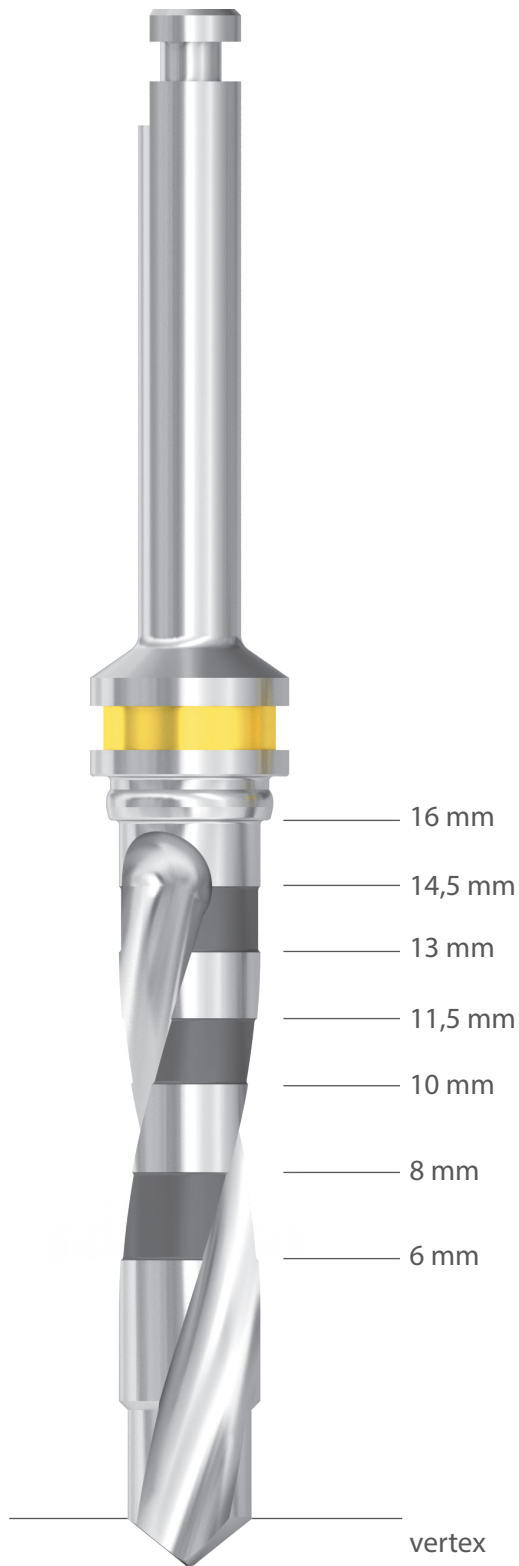

The BIONIKA drills - which can be used during implant insertion - are available in a wide range of sizes (compatible with different instrument kits to provide you with the most economical solution).

Our drills are externally cooled and have bone collecting properties. Acidic alloy steel and excellent sharpness guarantee long-term use. Each drill is provided with the required drilling depths. Diameters are indicated by color codes.

Spiral drills are suitable for preparing implant nests. They are recommended to use according to the drilling protocol, in the case softer and harder bone structures.

The Thread Calibrator Drills are suitable for expanding the implant nests as needed, so that we can extend the upper third of the bone nest. They are recommended to use in the case of harder than average bone structure.

The sizes available of the surgical drills in the instrument kit

SPEAR-POINTED DRILL ▼



PRE-DRILL Ø2,0 mm ▼



PRE-DRILL Ø2,5 mm ▼



PRE-DRILL Ø2.7 mm ▼



CORE DRILL Ø2,8 mm ▼



THREAD GROOVE CALIBRATION DRILL Ø3,2 mm ▼




CORE DRILL Ø3,2 mm ▼



THREAD GROOVE CALIBRATION DRILL Ø3,7 mm ▼



CORE DRILL Ø3,7 mm ▼



THREAD GROOVE CALIBRATION DRILL Ø4,2 mm ▼



CORE DRILL Ø4,2 mm ▼




THREAD GROOVE CALIBRATION DRILL Ø4,7 mm ▼



CORE DRILL Ø4,7 mm ▼



THREAD GROOVE CALIBRATION DRILL Ø5,2 mm ▼




Ratchet torque wrench

The ratchet torque wrench is used to tighten and insert screws and implants. Using pre-set torque, this prevents the implant from fracturing and ensures the optimum power transfer when inserting the implant.


The scale of the torque rates from 15 to 35 Ncm. The desired torques can be adjusted from 15 Ncm to the right for the desired scale.

When the ratchet torque wrench adjuster screw bolted to the stop, the wrench of the torque can be infinite, so it can also be used to produce a much greater torque than the torque shown on the scale, as needed.

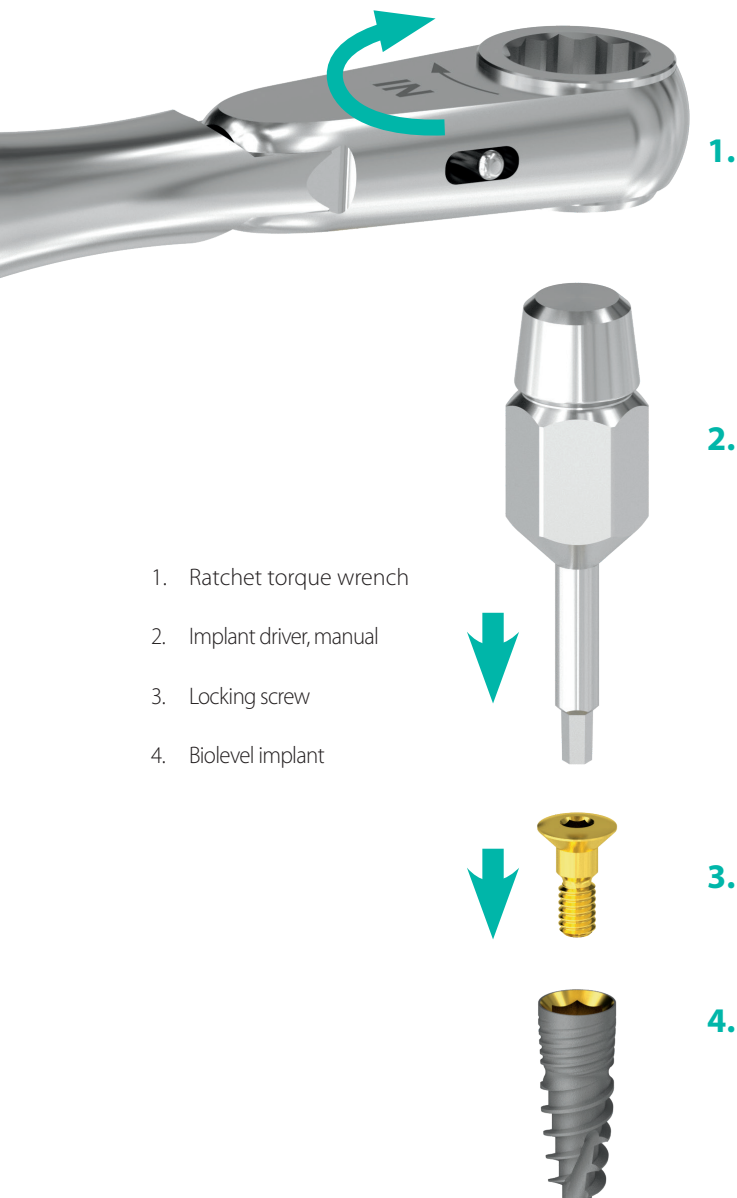

- ERGONOMIC CONSTRUCTION
- RELIABLE LIFETIME
- PRECISE TORQUE CONTROL
- STAINLESS STEEL
- SOUND SIGNAL
- REPLACABLE KEY INTERLINE
- STABLE TORQUE SCALE DURING USE
- PROFESSIONAL QUALITY









15 Ncm
25 Ncm
35 Ncm
endless torque



The desired torques can be adjusted from 15 Ncm to the right.

The applications of ratchet torque wrench



Heads and Screws		Key Interline	Torque
Locking screw			Manual key driver 10-15 Ncm
Healing cap			
Sampling head screw for closed and open spoon			
Sampling head for closed and open spoon			
Head screw			Ratchet torque wrench Torque of the required screw tightening: In the case of M1,4 screw it is 15 Ncm In the case of M1,6 screw it is 20 Ncm In the case of M1,8 screw it is 25 Ncm In the case of M2,0 screw it is 30 Ncm
Universal head, straight			
Universal head, oblique			
Anatomical head, straight			
Anatomical head, oblique			
Titanium base			
Multi-unit head, through-bolted			
Multi-unit head screw, SR-head screw			
Multi-unit head, screwable			
SR-head, screwable			
Ball-head			
Locator head			



Get to know our other products!

Ask for our catalogs or visit one of our websites below:



www.bionika.hu



www.shop.bionika.hu

