

## IMPLIE System selections of abutments


Implant diameters and color codes:			
IN	∅ 3,2	∅ 3,5	
IS	∅ 3,75	∅ 4,2	∅ 5,0

	Denomination	Sulkus (mm)	Height (mm)
1	Locking screw	-	-
2	Healing cap, narrow	2 4 6	-
3	Healing cap, anatomical	2 4 6	-
4	Technical implant		12
5	Sampling head for closed spoon		11
6	Sampling head for open spoon		11
7	Castable plastic head, Co-Cr based positioned		12
8	Castable plastic head, Co-Cr based, non-positioned		12
9	Interface, positioned	-	-
10	Interface, non-positioned	-	-
11	Temporary head, positioned		12
12	Temporary head, non-positioned		12
13	Temporary head, positioned, PEEK		12
14	Temporary head, non-positioned, PEEK		12
15	Narrow head, straight		9
16	Narrow head, 15°, 25° oblique		9
17	Universal head, straight		11
18	Universal head, 15°, 25°, 25°, 45° oblique		11
19	Anatomical head, straight	2 4 6	
20	Anatomical head, 15°, 25° oblique	2 4 6	
21	Trapezoidal head 15°, 25°, 35°, 45°		9 11 13
22	Delta head 15°, 25°, 35°, 45°		9 11 13
23	Titanium base		5
24	Press ceramic base		5
25	Tube head, positioned		9
26	Tube head, non-positioned		9
27	Scanbody head, through-bolted		12
28	Scanbody head, screwable		12
29	Ball head	0,5 1 2 3 4 5 6 7	
30	Locator head, straight	0,5 1 2 3 4 5 6 7	
31	Multi-unit head, straight	0,5 1 2 3 4 5 6 7	
32	Multi-unit head, through-bolted	0,5 1 2 3 4 5 6 7	
33	Multi-unit head, 20°, 30° oblique	1 2 3 4 5 6 7	
34	Multi-Compat head, 20°, 30° oblique	1 2 3 4 5 6 7	
35	Multi-unit SR head, straight	0,5 1 2 3 4 5 6 7	
36	Multi-unit SR head, through-bolted	0,5 1 2 3 4 5 6 7	
37	Multi-unit SR head, 20°, 30° oblique	1 2 3 4 5 6 7	
38	OC metal cap, OC plastic insert, 1,8 ; 2,5	-	-
39	Locator cap set	-	-
40	Castable plastic head, plastic, Multi-unit	-	-
41	Castable plastic head, Co-Cr based, Multi-unit	-	-
42	Castable plastic head, titan based, Multi-unit	-	-
43	Castable plastic head, Multi-unit SR	-	-
44	Castable plastic head, Co-Cr based, Multi-unit SR	-	-
45	Castable plastic head, titan based, Multi-unit SR	-	-

Sizes can be varied according to unique requests.

## The functional structure of the IMPLIE system elements

Grade 4 quality titanium is applied in the case of the implants and Grade 5 quality titanium is applied in the case of the abutments. Our abutments can be made of Co-Cr material and POM or PEEK materials are applied in the case of plastic heads.


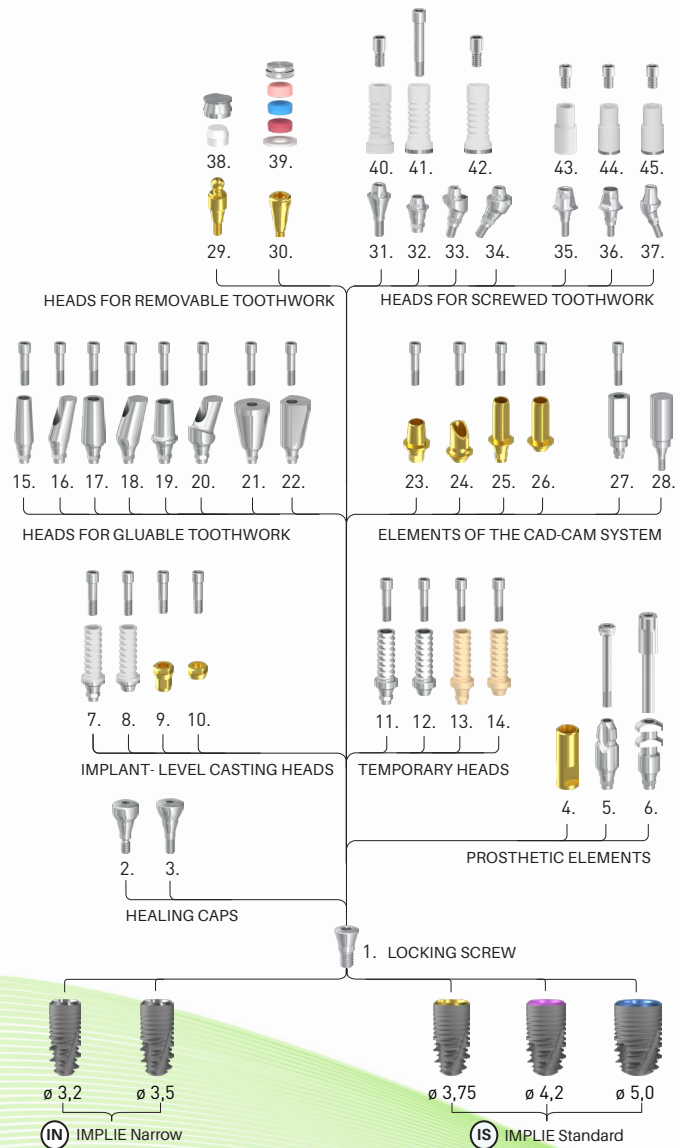


K21-MD07-006

# BIONIKA

# IMPLIE

## Implant System

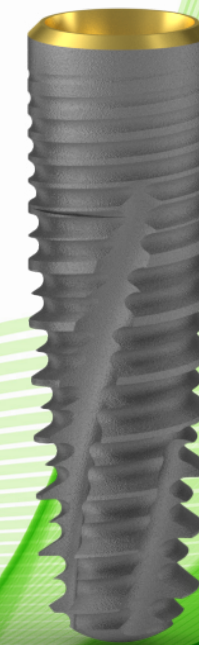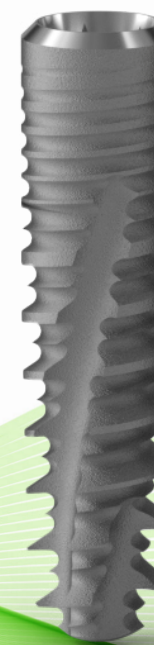

BIONIKA Medline Kft. • 3516 Miskolc, Téglá u. 29.  
[www.bionika.hu](http://www.bionika.hu) • [info@bionika.hu](mailto:info@bionika.hu)  
**mobil: + 36 70 670 6875**

The products in the publication are only illustrations, they do not cover the exact appearance and shape of the product.

## Company

BIONIKA Medline Medicaltechnics Ltd. was formed in 1989. We have more than 30 years of experience in developing, manufacturing and sales of surgical instruments and implants.

BIONIKA is present in the technical fields of odontology, oral surgery, traumatology, orthopaedics and rehabilitation as a company dealing with research and development as well as manufacturing and distribution.

According to our aim and conception we attach great significance to the word „BIONIKA“ that represents a scientific way of thinking along the common borderlines of biology, technology and electronics, which combines these three fields during our work of research and development.



### Clinical and technological experience:

Clinical and technological experiences: Continuous process, combination and utilisation of the clinical and technological experiences in development contribute to our success, with a feedback throughout the manufacturing base. The most adequate solutions and constructions satisfying the customer demands are born here and they are continuously developed.

**Development:** Owners of BIONIKA attach great importance on continuous product and technological development. Our products are developed by close co-operation of doctors and engineers, fact by which we can assure the highest quality available worldwide and practical efficiency at the same time.

**Quality:** The design, manufacturing and quality management performed according to the adopted measures of the European Union assure the quality expected by our Customers. The BIONIKA Medline Ltd. works according to the EN ISO 9001 and ISO 13485 quality management systems. Our products are marked with the CE sign.

**Warranty:** Following the implantation process, we provide warranty for replacing the unit within one year counting from the date of purchase, regardless of the causal relevance. BIONIKA assumes the risk of ossification process. Otherwise we provide a 10-year long-term warranty for our products.

## Specifications of the IMPLIE Implant System

In the dental and implantological practice among the existing ones there is a new demand for simple implant system which covers the patients with average bone structure. It's main characteristics that it's better in following the biological root form and the structure of the primer stable thread has been researched using the latest technologies and the construction offers the highest primer stability which accomodates well with both the corticalis and the spongiosa jaw structure due to our 30 year experience. That's how the IMPLIE Implant Family have been researched.



### Connection: Cone & Hex

This complex cone & hexagonal prism geometry has been proved in the engineering practice and ensures the perfect fitting. We are using a 25-degree cone angle that provides a micro move-free load transmission and assures good conditions for accurate open or closed tray method. It superimposes the forces deep into the implant's inside.

### Platform switching

The fitting diameter of the abutment is smaller than the outside part of the implant connecting to the bone. The bone may slide on to the top flange of the implant, and in turn the soft tissue will close in around the ingoing aperture of the bone nest and the implant's connecting surface, covering and sealing it up like a sealing ring.

### Spiral, micro-grooved corticalis surface:

Holding on to the corticalis, the multi-start micro-grooved spiral surface functions as a significant load-bearing element both in the primary and later stage. Due to the cycloid knuckle thread geometry, this selflocking thread structure facilitates deducting the dynamic effects and facilitates the micro move-free conditions and assures a fast incorporation.

### Anatomical tooth root-shape, high pitch selfcompressing spongiosa thread:

The IMPLIE follows the anatomical shape of the root. Due to the epsilon thread profile, the tapered thread and the high pitch, large thread depth, and the self-locking and self-cutting formation of the implant, it has a bone-compacting effect. As a result of the high primary stability, this enables the implant to be promptly loadable if needed.

### Rounded implant end:


It facilitates the smaller direction changes during the implant insertion.




## The parameters of the IMPLIE Implant System

diameter (mm)	implant length (mm)				
	8	10	11,5	13	16
ø 3,2	○	○	○	○	○
ø 3,5	●	●	●	●	●
ø 3,75	●	●	●	●	●
ø 4,2	●	●	●	●	●
ø 5,0	●	●	●	●	●


### ø 3,2

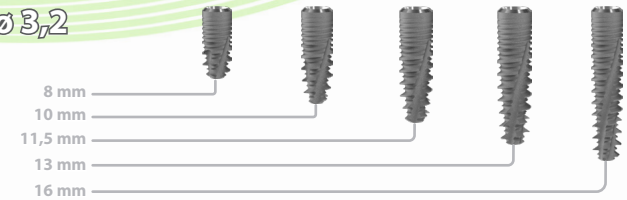


### ø 3,5

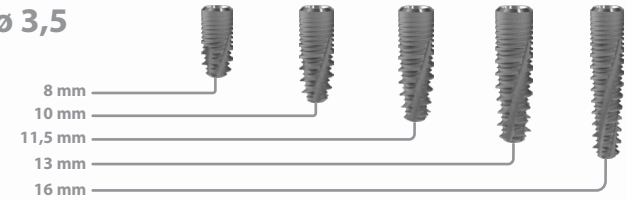

### ø 3,75

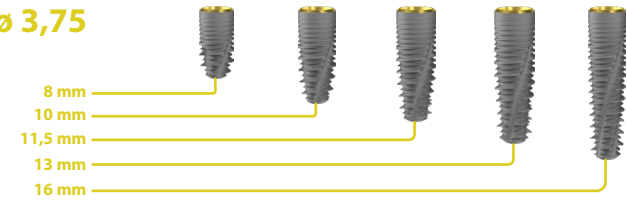

### ø 4,2

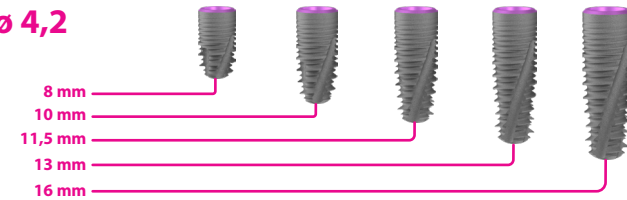

### ø 5,0

